# ΗΙΟΚΙ

# MEMORY HICORDER MR6000

MR6000

HICORDER



нюкі

# Exceed All Limits

Fast and powerful - the best specs in the history of Memory HiCorders

Best-in-Class Flagship Model

Measurement	Blazing fast, never-fail sampling High-speed isolation measurement at 200 MS/s
Storage	Superior processing capacity lets you save data while measuring Save data in real time, 32 times faster than conventional models
Usability	User-friendly design for accurate and smooth operation Intuitive operation via large 12.1-inch touch screen



# Overwhelming high speed technology A revolutionary approach to measurement, recording and analysis

## MEMORY HICORDER MR6000

The MR6000 overcomes all barriers to reach new ground and meet challenges that are yet to be seen. World class specifications, operability and design - Hioki's newest memory recorder has been re-engineered from top to bottom, delivering unprecedented performance that will change how you look at waveform recording. Redefining the world standard for recorders - that is the Hioki MR6000.

# 200MS/s

High-speed optical isolated measurement

## Instant saving Real-time save

Intuitive operation




Increased efficiency of inverters and improved performance of energy-saving technologies have been achieved in the power electronics, renewable energy, and automotive industries. We have drastically improved the technology used in our Memory HiCorders, developing the MR6000 Memory HiCorder to meet the advanced demands of all industries.



# Series-Leading Measurement Performance

## High-speed isolated measurement at 200 MS/s Up to 32 ch in the analog unit and up to 128 ch in the logic unit

The Hioki Memory HiCorder lineup now includes a powerful input unit that unlocks the full measuring potential of the MR6000. The High Speed Analog Unit U8976 boasts the highest sampling rate in its entire series, an order of magnitude faster than conventional models, enabling the unit to perform isolated measurement at 200 MS/s°. Combine multiple modules of the 4ch Analog Unit U8975, which provides 4 channels of input with a speed of 5 MS/s at 16 bits, to perform multi-channel measurements up to 32 channels. Make the most of the Memory HiCorder's capabilities as we continue its development to meet your advanced measurement needs.



200 MS/s measurements can be achieved even if a unit other than the U8976 is connected at the same time. However, the data update rate will not exceed the maximum sampling rate of the unit.

#### Blazing fast, never-fail sampling Record high-precision waveforms



#### HIGH SPEED ANALOG UNIT U8976

You need accurate detection of switching waveforms in inverter evaluation tests, which requires a high level of efficiency. We developed the High Speed Analog Unit U8976 to meet those needs. In addition to high-speed sampling at 200 MS/s, the unit supports frequency bands up to 30 MHz. Adapted to the Memory HiCorder's direct input feature, it supports inputs up to 400 V DC.

Available recor duration	ding		5-second recording		
Sampling rate	1 ch	2 ch	3 to 4 ch	5 to 8 ch	9 to 16 ch
200 MS/s	5 s	2.5 s	1 s	0.5 s	0.25 s
100 MS/s	10 s	5 s	2 s	1 s	0.5 s
50 MS/s	20 s	10 s	4 s	2 s	1 s
20 MS/s	50 s	25 s	10 s	5 s	2.5 s
:	:	:	:	÷	:
· · ·					


\* Internal memory used \* U8976 installed in 8 slots

### Install up to 8 units with 4 channels each Measure multiple points simultaneously




4CH ANALOG UNIT U8975 4CH ANALOG UNIT U8978

Our lineup now includes two types of analog units with 4-channel input in a single device. The U8975 supports direct inputs up to 200 V DC, and the U8978 is effective for accurately capturing sensor output using its 100 mV f.s. high sensitivity range. Both units provide a sampling rate of 5 MHz and 16-bit resolution



Conventional sampling (20 MS/s)




## 200 MS/s High-speed sampling



#### Isolated input with optical isolation devices

Connections between analog input channels, and between the input channel and the main unit, are fully isolated. This means that, unlike an oscilloscope, measurements can be made without concern with negative effects from potential differences

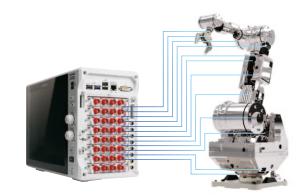

Simultaneous measurement of multiple locations across 32 channels at 5 MS/s



# A rich unit lineup for detecting a wide range of phenomena

Combine multiple units to record a range of phenomena. A high-voltage unit with a direct input of 1000 V DC is ideal for measuring global power lines, including uninterruptible power supplies (UPS) and commercial power supplies. Use multiple logic units to measure relay ON/OFF signals or PLC (programmable logic controller) signals across up to 128 channels simultaneously.

Unit interchangeability

The unit types compatible with the MR6000 are identical to the ones compatible with the MEMORY HiCORDER MR8827, MR8847A, MR8740, MR8741, and MR8740-50. Use any of the 15 types listed in the unit selection guide below. However, the U8977, U8978, and U8979 can only be used with the MR6000.

		Jii gu		500)							av		ver 2.10 of late
	Measured signal	Model	Description	No. of channels	Fastest sampling	Bandwidth	A/D resolution	DC accuracy	Max. input voltage	Sensitivity (#1)	Max. sensitivity range	Isolation	Supplement
	Voltage (high speed)	U8976	High-Speed Analog Unit	2 ch	200 MS/s	DC to 30 MHz	12 bits	±0.5% f.s.	400 V DC 1000 V DC (#2)	0.0625 mV	100 mV f.s.	Yes	n/a
	Voltage	8966	Analog Unit	2 ch	20 MS/s	DC to 5 MHz	12 bits	±0.5% f.s.	400 V DC	0.05 mV	100 mV f.s.	Yes	n/a
	Voltage (4ch)	U8975	4ch Analog Unit	4 ch	5 MS/s	DC to 2 MHz	16 bits	±0.1% f.s.	200 V DC	0.125 mV	4 V f.s.	Yes	n/a
NEW	Voltage (4ch, high resolution)	U8978	4ch Analog Unit	4 ch	5 MS/s	DC to 2 MHz	16 bits	±0.3% f.s.	40 V DC	3.125 uV	100 mV f.s.	Yes	n/a
	Voltage (high resolution)	8968	High Resolution Unit	2 ch	1 MS/s	DC to 100 kHz	16 bits	±0.3% f.s.	400 V DC	3.125 uV	100 mV f.s.	Yes	with AAF
	Voltage (DC, RMS)	8972	DC/RMS Unit	2 ch	1 MS/s	DC to 400 kHz	12 bits	±0.5% f.s.	400 V DC	0.05 mV	100 mV f.s.	Yes	with RMS
-	Voltage (high voltage)	U8974	High Voltage Unit	2 ch	1 MS/s	DC to 100 kHz	16 bits	±0.25% f.s.	1000 V DC 700 V AC	0.125 mV	4 V f.s.	Yes	CAT IV 600 V AC/DC
	Voltage (high resolution)	MR8990	Digital Voltmeter Unit	2 ch	2 ms	n/a	24 bits	±0.01% rdg. ±0.0025% f.s.	500 V DC	0.1 uV	100 mV f.s.	Yes	CAT II 300 V AC/DC
NEW	Current	U8977	Current Unit	3ch	5 MS/s	DC to 2 MHz	16 bits	±0.3% f.s.	Current sensor only		on current nsor	n/a	Max. 3 Units
	Current	8971	Current Unit	2 ch	1 MS/s	DC to 100 kHz	12 bits	±0.65% f.s.	Current sensor only		on current nsor	n/a	with RMS Max. 4 Units
	Temperature	8967	Temperature Unit	2 ch	1.2 ms	DC	16 bits	Detailed reference	Thermocouples only	0.01°C	200°C (392°F)f.s.	Yes	n/a
	Strain	U8969	Strain Unit	2 ch	200 kS/s	DC to 20 kHz	16 bits	±0.5% f.s. ±4 με	Strain only	0.016 με	400 μεf.s.	Yes	n/a
	Frequency	8970	Frequency Unit	2 ch	200 kS/s	DC to 100 kHz (#3)	16 bits	n/a	400 V DC	0.002 Hz	Depends on mode	Yes	n/a
NEW	Acceleration	U8979	Charge Unit	2 ch	200 kS/s	DC to 50 kHz (DC) 1 Hz to 50 kHz (AC)	16 bits	±0.5% f.s. (Voltage) ±2.0% f.s. (Acceleration)	40 V DC		nds on tion sensor	Yes	Supports TEDS
	Logic	8973	Logic Unit	4 probes (16 ch)	n/a	n/a	n/a	n/a	n/a	n/a	n/a	n/a	Requires 9320-01, 9327 or MR9321-0

#### Unit selection guide (15 types)

(#1) Minimum resolution shows the highest sensitivity resolution. (#2) When using the 9665 (#3) Minimum pulse width 2 µs

available for Ver 2.10 or later


# Concentration of sensing technologies with superior accuracy: A rich set of functions suitable for all measuring purposes

Sensing technology that serves as the key to reliable measurement data is essential for detecting various phenomena across multiple channels. The MR6000 is a high-spec model that fully leverages the performance of Hioki's high-precision sensors.



## Compatible with high-precision sensors for measuring large currents

Combine the Current Unit (8971 or U8977) and a current probe or current sensor designed and manufactured by Hioki to use the system over a wide temperature range or measure large currents with a high level of precision at solar power plants or development sites for EVs/HEVs. The convenient, built-in sensor identification function lets you simply connect the sensor to easily configure the scaling settings through automatic recognition. Combine the High Speed Analog Unit U8976 and a Hioki current probe or clamp-on probe for high-precision wideband observation of current waveforms. Furthermore, install the optional Probe Power Unit Z5021 to drive these probes from the MR6000 main unit.



# Triggers that detect targeted events


Set triggers on any channel to record data whenever an event occurs.

Level trigger	Compares to one voltage value.
Window trigger	Compares to two voltage values.
Voltage drop trigger	Detects voltage drops in commercial power lines.
Period trigger	Monitors periods.
Glitch trigger	Detects anomalies in pulses.
Pattern trigger	Compares when the logic signal is ON/OFF.

### Setting multiple triggers for a single channel

Set up to 4 triggers for a single channel. If, for instance, you set the glitch, level, window-in, and window-out triggers for the same input waveform, that waveform is monitored according to the set trigger conditions.

Various triggers x Up to 4 Settable for any channel

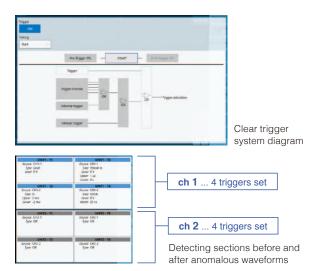


# Observe fluctuations over the long-term with high-speed sampling

The system uses the envelope measurement method to record maximum and minimum values at set intervals while performing oversampling at 100 MS/s. The internal memory has a capacity of 1 G-words, which ensures that the measuring process continues for a long time without any data losses. Save data in real time while measuring.

Oversampling speed	Recording intervals	1 ch	 9 to 16 ch
	10 MS/s	50 s	 2 s
	1 MS/s	8 m 20 s	 20 s
	100 kS/s	1 h 23 m 20 s	 3 m 20 s
100 MS/s	10 kS/s	13 h 53 m 20 s	 33 m 20 s
100 103/5	1 kS/s	5 d 18 h 53 m 20 s	 5 h 33 m 20 s
	-	:	
	20 S/s	289 d 8 h 26 m 40 s	 11 d 13 h 46 m 40 s
	:	:	 :

Limitations apply to measurable time when the U8975, U8977, U8978, or MR8990 is in use, and when performing real-time waveform processing.

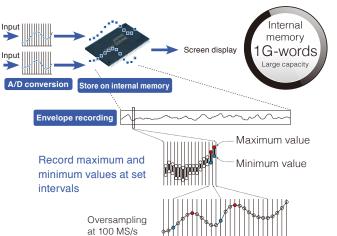

## Equipped with a powerful data analysis function

#### FFT calculation function (Equipped from Ver. 2.10)

NEW ALL Installed in MR6000, MR6000-01

Analyze 8 phenomena at the same time with a single measurement. Multiple FFT analyses of signals input from different channels let you investigate the frequency components that appeared for each channel at a single point in time. Similarly, conduct a variety of analyses for a single signal simultaneously.

-	Sampling	Points	-	Recording time Mode
9	20 MS/s	2.5 k	Any	125 µa Single V Read
2				Simultaneous analyses a display of 8 phenomena
				Cursor-
				1.2MHz 1.6MHz Calc
	00mV			RMS spectrum (CH1-1)
				Gauge
ņ				FFT3
OF		400kHz	800kHz	Overall 555.8832mV
5) #				Power spectrum (CH1-1) Charnel post on post on post of post on post of post of
ķ				FFT5 Auto range
		400kHz	800kHz	Overall 309.0061mV2 FFT6
11				Linear spectrum (CH1-1)
				Overall 555.8832mV

FFT calculation 4-split screen

# Waveform processing function (Equipped from Ver. 2.10) NEW ALL Installed in MR6000, MR6000-01

Perform complex calculations using previously loaded waveforms. Make up to 16 calculations, including logarithmic conversions, various filters, and trigonometric functions, simultaneously. You can also compute the average value, maximum value, or minimum value of the loaded data and reuse the results in further waveform processing operations.

Z1	Comment	Half-wave rectification
On	Formula	(CH(1,1)+ABS(CH(1,1)))/2
Z2	Comment	Capacitance
ON	Formula	INT(CH(2,1))/CH(2,2)
Z3	Comment	Inductance
Z3 ON		Inductance LPFIR(CH(3,1),500,200,10)/DIF(LPFFIR(CH(3,2),500,200,10))

Supports complex calculations

#### Real-time waveform processing

#### ONLY Installed in MR6000-01

#### Calculate measurement data during measurement

The MR6000-01 further features a powerful technology designed for robust real-time waveform processing. This function performs the four arithmetic operations (addition, subtraction, multiplication, and division), differentiation calculations, or integration calculations during the measuring process, letting you use check the calculated results via waveforms while measuring. Results can be further processed after measurement and saved.

	W1	Comment	addition	
	On	Formula	(CH(1, 1)) + (CH(1, 1))	
		Comment	sabtraction	
	On	Formula	(CH(1, 1)) - (CH(1, 1))	
ļ	W3	Comment	multiplication	
			multiplication (CH(1, 1)) x (CH(1, 1))	

Simple setting method



Dedicated equipment installed only in the MR6000-01 for realtime waveform processing

#### FFT analysis directly from the memory waveform

Perform FFT analysis from measured data. Simply touch the screen to specify the starting point for analysis, while simultaneously viewing the calculation results.



Chronological order + FFT calculation screen

#### Numerical calculation function

ALL Installed in MR6000, MR6000-01

Analyze measured waveforms with numerical parameters. The MR6000 features several new numerical calculation functions including those for identifying overshoot and undershoot. In addition to analog and logic channels, the MR6000 can also perform calculations on real-time waveform processing channels, and features a numerical comparator function.


Average value	Average value Rise time		Amplitude
RMS value	Fall time	Pulse count	Overshoot
Peak to peak value	Standard deviation	Four arithmetic operations	Undershoot
Maximum value	Area value	Time difference	+Width
Time to maximum value	X-Y area value	Phase difference	-Width
Minimum value	Specified level time	High-level	Burst width
Time to minimum value	Specified time level	Low-level	Integration values
Period	Pulse width	Median value	XY waveform angle
Frequency			

Simultaneous calculations of up to 16 out of a total of 33 computations

# Digital filter calculation

#### Observe clear waveforms without noise

Remove harmonic noise or specific frequency noise from measurement data. Use it to eliminate the noise that cannot be resolved with the standard filter installed in the unit.



Digital filter disabled

Digital filter enabled

# Highest Transfer Speed in the Entire Series


# Data transfer up to 32 times faster compared to conventional models Outstanding real-time save function that saves data during measurement

The MR6000 features a brand new interface that makes data transfer up to 32 times faster. In addition, faster internal processing allows data to be saved to external media in real time during measurement.



#### Drastically increased data transfer speed

Data transfer to storage devices is now up to 32 times faster. While conventional models transferred data at 1 MS/s in a single channel, the MR6000 transfers data for 32 channels.

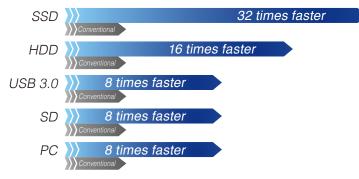

\*Compared to other recorders in the Hioki Memory HiCorder series. \*Results vary according to measurement conditions.

### Saving data directly to your PC

Transfer measurement data directly to your PC by using the FTP sending function together with the real-time save function. This makes it easier to observe data after the measuring process.



# Longest Continuous Recording in the Entire Series

# Long-term recording and high-speed sampling in multiple channels All in a single measurement

The real-time save function controls the available measurement duration without relying on the capacity of the internal storage memory. For long-term recording, we recommend a high-capacity SSD or HD unit. You can also use a more convenient USB memory stick or SD memory card. All phenomena can be recorded at a high sampling rate over a long period of time. This feature is ideal for situations where it is hard to predict the nature of a phenomenon or for measurements that can only be performed once. When saved in real time, data is split into several 512 MB files.



d: days h: hours min: minutes s: seconds

#### Available real-time save duration for various media

Save destination	Sampling speed	Number of channels	Available measurement duration	Maximum sampling rate for real-time save *1
SSD UNIT U8332 (256 GB)	1 MS/s	32 ch	Approx. 1 h	20 MS/s
HD UNIT U8333 (320 GB)	1 MS/s	16 ch	Approx. 2 h 40 min	10 MS/s
USB DRIVE Z4006 (16 GB)	1 MS/s	8 ch	Approx. 16 min	5 MS/s *2
SD MEMORY CARD Z4003 (8 GB)	1 MS/s	8 ch	Approx. 8 min	5 MS/s
PC	1 MS/s	8 ch	Depends on PC capacity	5 MS/s


\*1: For 2 channels (no settings for 1 channel) \*2: When using the USB 3.0 connector

# Maximum recording duration for real-time save with an SSD UNIT U8332/Reference values

Sampling		Nu	mber of channels us	ed	
rate	2	4	8	16	32
20 MS/s	53 min 20 s	-	-	-	-
10 MS/s	1 h 46 min 40 s	53 min 20 s	-	-	-
5 MS/s	3 h 33 min 20 s	1 h 46 min 40 s	53 min 20 s	-	-
2 MS/s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s	-
1 MS/s	17 h 46 min 40 s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s	1 h 6 min 40 s
500 kS/s	1 d 11 h 33 min 20 s	17 h 46 min 40 s	8 h 53 min 20 s	4 h 26 min 40 s	2 h 13 min 20 s
200 kS/s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s	5 h 33 min 20 s
100 kS/s	7 d 9 h 46 min 40 s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s	11 h 6 min 40 s
50 kS/s	14 d 19 h 33 min 20 s	7 d 9 h 46 min 40 s	3 d 16 h 53 min 20 s	1 d 20 h 26 min 40 s	22 h 13 min 20 s
20 kS/s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9d6h13min20s	4 d 15 h 6 min 40 s	2 d 7 h 33 min 20 s
10 kS/s	74 d 1 h 46 min 40 s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9 d 6 h 13 min 20 s	4 d 15 h 6 min 40 s
5 kS/s	148 d 3 h 33 min 20 s	74 d 1 h 46 min 40 s	37 d 0 h 53 min 20 s	18 d 12 h 26 min 40 s	9d6h13min20s
2 kS/s	:	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s	23 d 3 h 33 min 20 s
1 kS/s		:	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s	46 d 7 h 6 min 40 s
500 S/s			:	185 d 4 h 26 min 40 s	92 d 14 h 13 min 20 s
200 S/s				:	231 d 11 h 33 min 20 s
100 S/s					:

# Long-term measurements for more efficient testing

The real-time save function boasts high-speed sampling and multi-channel measurements. Perform an approximately 1-hour measurement at 20 MS/s in 2 channels or 1 MS/s in 32 channels.



HIOKI

Ø 14:45:07.583

50 KS/

# User-Friendly Flexible Design

# Fast and convenient touch screen Operation as smooth as silk

The capacitive touch screen delivers intuitive operability.

Select a setting item directly by tapping the screen, and use your fingers to enlarge the part you want to see.

The new user interface makes setting measurement items for multiple channels easier compared to the more complicated conventional models where you had to press the keys several times to configure a setting.



▲ Use the rotary knobs to move the tracing cursor.



Touch screen 12.1 inches

Large LCD

0

▲ Simply tap the screen to switch between the items you want to set.

# Easy method for pinpointing a specific waveform within large amounts of measurement data

Set the peak values or trigger conditions you want to search for to have the relevant data retrieved and displayed automatically. Our new Memory HiCorder Concierge function automatically calculates the characteristics of the reference waveform you have set and searches all of the measured data to detect and array any waveforms with low similarity as anomalous waveforms. This drastically reduces the amount of time required to search for anomalies by eliminating the need to scroll through measured waveforms and check them visually.

## Memory HiCorder Concierge

#### Use the Concierge to look for anomalous waveforms.

A new waveform search function finds anomalous waveforms in all of the measured data. This function is ideal for situations where it is difficult to set the right triggers before measuring because the nature of potential anomalies cannot be predicted.

Automatically search for waveforms with low similarity to the reference waveform

### Rich set of search functions

Registering a reference waveform

#### Peak search

Search for the maximum value, minimum value, local maxima, or local minima in all of the measured data, and mark the search point in the waveform.

#### Trigger search

Set trigger conditions for all of the measured data again to search for points where the conditions are fulfilled, even if no triggers were set during the measuring process.

#### Jump

New function Waveform

Search Automatically search

for anomalous


waveforms

Jump to an event mark you made while measuring, to the cursor position on the display, or to the location measured at a specified time.

## Radically improved data saving time

Transferring very large amounts of data measured over a long period of time used to be very time-consuming. The MR6000 features a brand new interface and faster internal processing, reducing the time required to save measurement data to media. This saves you the trouble of waiting for data to be saved and improves work efficiency.


USB 2.0	Existing models	
036 2.0	MR6000	Reduced to 1/5
USB 3.0	MHOUUU	<ul> <li>Further reduced to 1/10</li> </ul>
HD	Existing models	
ПD	MR6000	<ul> <li>Reduced to 1/20</li> </ul>
SSD	MROUUU	<ul> <li>Further reduced to 1/30</li> </ul>

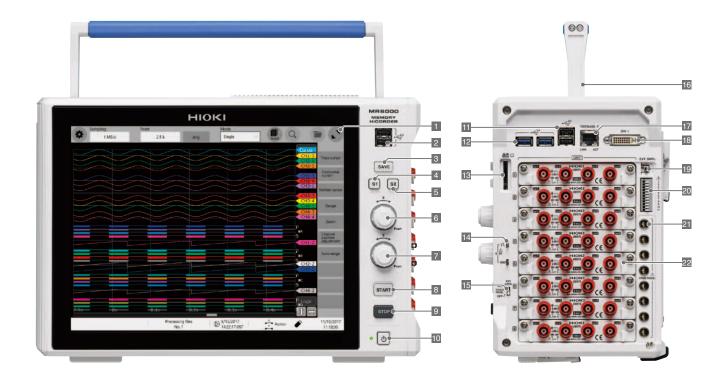

# Multifunctional Interface


# Only 6 keys in total New recorder design

Use the touch screen to configure all the basic settings.

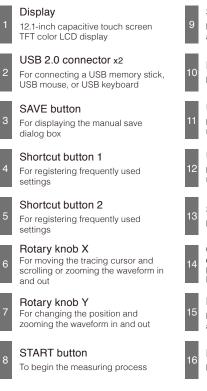



Open or close the top panel of the main unit. Z4006 USB DRIVE installable.

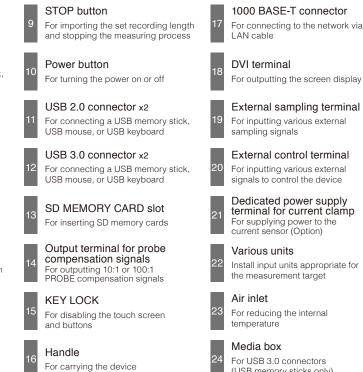

- **DVI** terminal For outputting the screen display External sampling terminal For inputting various external sampling signals
- External control terminal For inputting various external signals to control the device

Dedicated power supply terminal for current clamp For supplying power to the current sensor (Option)

Various units Install input units appropriate for the measurement target

For reducing the internal

For USB 3.0 connectors (USB memory sticks only)

# Operability and visibility suited for a variety of work environments

## Ergonomical operating angle

Our search for a touch screen with the best operability and visibility angle led us to develop retractable feet that maximize those two important attributes. Tilting the MR6000 with the feet reduces the strain on your wrists when you use the device on a desk, and keeps your line of sight at a natural level. The rear side also features the same retractable feet, making is easy to use the device on the floor.



## Space-saving size

We have achieved a design that is compact while still delivering blazing fast processing speeds by using thermal liquid analysis to optimally position the air inlets, heating components, and cooling fans. The smaller form factor requires less space for installation, making the device just right for tight workspaces.

# Sleek details

HIOKI

Easy multi-touch

Horizontal and vertical

When compared to 8861-50



# Easy handling

The rubber handle boasts excellent grip and makes it easy to carry the device with either one or both hands. The grips on either side of the device can also be used to lift it with both hands.

Simple protectors on the top and bottom right side of the device protect the interface and unit input terminals from sudden physical shocks.

Refined attractive shape

The bevelled chassis edges give the device a compact and sleek look. The left side is slightly curved with slits to match the mesh of the air outlet. The air outlet is therefore in harmony with the design of the flat and solid-looking chassis. The simple and refined appearance achieved by these efforts well suits a device used for R&D purposes.

# Product Specifications

(Accuracy guaranteed for			
	Normal: Regular wa	nt accuracy guaranteed for 1 year) veform recording	
Recording method	*Envelope setting no	Ily recording maximum and minimum values ot available with external sampling 2 channels (with 4ch ANALOG UNIT U8975/U8978)	
No. of channels	Logic with up to 128 *Common GND for t	channels (LOGIC UNIT 8973) the logic probe input connector and main unit	
Maximum sampling rate	200 MS/s (all chann U8976) External sampling ( <sup>-</sup>	els at the same time) (with HIGH SPEED ANALOG UNIT	
Memory capacity	1 G-words		
Operating environment	Indoors, pollution degree 2, altitude up to 2000 m (6562.20 ft)		
Operating temperature and humidity range	0°C to 40°C (32°F to	o 104°F), 80% RH or less (no condensation)	
Storage temperature	-10°C to 50°C (14°F	to 122°F), 80% RH or less (no condensation)	
and humidity range Compliance standards	Safety: EN61010, El		
Power supply	for rated supply volt	e: AC 100 V to 240 V (consider ±10% voltage fluctuations age) frequency: 50 Hz / 60 Hz	
Max. power consumption		t overvoltage: 2500 V	
Clock		-year correcting 24-hour clock	
Backup battery life PC interface (overview)	Approx. 10 years (at LAN, USB, SD, SAT	23°C (73°F)) for clock and settings	
External dimensions		235 mm (9.25 in) H x 154.8 mm (6.09 in) D (excluding protrusions)	
Mass	6.5 kg (229.3 oz) (m 6.7 kg (236.3 oz) (w 8 9 kg (313 9 oz) (w	ain unit only) ith Z5021, U8332, or U8333 installed) th HIGH SPEED ANALOG UNIT U8976 installed)	
Accessories	Power cord, Quick Sta application disk (CD-F	rt Manual (booklet, CD-R), operating precautions (booklet), R), Instruction Manual (detailed edition) (CD-R), Instruction	
Accuracy	Manual (MR6000-01 e	exclusive functions edition) (CD-R), blank panel (blank slot only)	
Accuracy guarantee	Temperature and bu	midity range: 23°C ±5°C (73°F ±9°F), 80% RH or less	
conditions Time axis accuracy	±0.0005%		
Display			
Display type	12.1 inch XGA TFT c	olor LCD (1024 x 768 dots) with capacitive touch screen	
LAN Interface			
Compatibility specifications Functions		1000BASE-T, 100BASE-TX, 10BASE-T TTP, e-mail sending function	
Connector	RJ-45		
Maximum cable length	100 m (328.11 ft)		
USB interface Compatibility specifications	USB 3.0 compliants	< 3, USB 2.0 compliant x 4	
Host	Connector: Series A	receptacle	
Available options	Connected devices Z4006 USB MEMOR	: Keyboard, mouse, USB memory stick RY STICK (16 GB)	
SD card slot			
Compatibility specifications		ndards x 1 (compatible with SD, SDHC, SDXC memory cards)	
Available options SATA interface	24001 SD MEMORY C	CARD (2 GB), Z4003 SD MEMORY CARD (8 GB)	
Compatibility specifications	Serial ATA Revision	3.0 compliant x 1	
Available options Monitor output	U8332 SSD UNIT (2	56 GB), U8333 HD UNIT (320 GB)	
Connector	DVI-I Digital output for exte	rnal dienlaue 1024 y 769 (VCA) *Not compatible with a 18-1	
Output type		rnal displays 1024 x 768 (XGA) *Not compatible with dual link	
Connector	terminal SMB 10 V DC		
Connector Maximum input voltage Input voltage	SMB 10 V DC 2.5 V to 10 V for high	n level, 0 V to 0.8 V for low level	
Connector Maximum input voltage Input voltage Response pulse width	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during	n level, 0 V to 0.8 V for low level g high periods, 50 ns or more during low periods	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during 10 MHz		
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during 10 MHz External sampling c rminals	g high periods, 50 ns or more during low periods	
External sampling Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during 10 MHz External sampling c rminals Push-button type	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during 10 MHz External sampling c rminals	g high periods, 50 ns or more during low periods	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block	SMB 10 V DC 2.5 V to 10 V for higj 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods.	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block	SMB 10 V DC 2.5 V to 10 V for higj 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods.	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling o <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Founctions Output type	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output)	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for high 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling o <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Founctions Output type	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage Maximum input voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors,	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Gutput type Output voltage Maximum input voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Response pulse width Pulse interval Number of terminals Functions Output voltage Maximum input voltage Number of terminals Functions	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Mumber of terminals Functions Mumber of terminals Functorions Maximum input voltage Maximum input voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods	
Connector Maximum input voltage Mesponse pulse width Maximum input frequency Functions External control te Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling o <b>rminals</b> Push-button type Maximum input voltage Input voltage Maximum input voltage Maximum input voltage Maximum input voltage Maximum input voltage Kumber of terminals Functions Maximum input voltage Response pulse	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF; 1 ms or more during high periods, 2.5 ms or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2.5 ms or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2.5 ms or more during low periods	
Connector Maximum input voltage Mesponse pulse width Maximum input frequency Functions External control te Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling o <b>rminals</b> Push-button type Maximum input voltage Input voltage Maximum input voltage Maximum input voltage Maximum input voltage Maximum input voltage Kumber of terminals Functions Maximum input voltage Maximum input voltage External trigger filter Response pulse	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2.5 ms or more during low periods Rising/falling selection possible Rising/falling selection possible	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling o <b>rminals</b> Push-button type Maximum input voltage Input voltage Maximum input voltage Maximum input voltage Maximum input voltage Maximum input voltage Kumber of terminals Functions Maximum input voltage Maximum input voltage External trigger filter Response pulse	a high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods Rising/Taling selection possible Rising: Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V).	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling or <b>rminals</b> Push-button type Input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage Maximum input voltage Maximum input voltage External trigger filter Response pulse width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 is or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V). Falling: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to w(0 V to 0.8 V) or when a terminal short circuit occurs.	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling or <b>rminals</b> Push-button type Input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage Maximum input voltage Maximum input voltage External trigger filter Response pulse width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 25 ms or more zuring low periods Rising: Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V), Falling: Triggering occurs. *Trigger filme; With the START&STOP option, rising/	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling or <b>rminals</b> Push-button type Input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage Maximum input voltage Maximum input voltage External trigger filter Response pulse width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 is or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V). Falling: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to w(0 V to 0.8 V) or when a terminal short circuit occurs.	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c minals Push-button type Input voltage Input voltage Number of terminals Functions Output type Output voltage Kaximum input voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2 us or more during low periods Rising. Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V), Falling: Triggering occurs. *Trigger filter START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level	
Connector Maximum input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c <b>rminals</b> Push-button type Maximum input voltage Input voltage Response pulse width Pulse interval Number of terminals Functions Output type Output voltage Response pulse width Functions Output type	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2.5 ms or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2.5 ms or more during low periods Rising/Triggering occurs when the voltage rises from New (0 V to 0.8 V) to high (2.5 V to 10 V). Palling: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to low (0 V to 0.8 V) or when a terminal short circuit occurs. *Trigger timing: With the STARTASTOP option, rising/ Trigger iming: With the STARTASTOP option, rising/ Trigger iming: With the STARTASTOP option, rising/ Trigger iming: With the STARTASTOP option, rising/	
Connector Maximum input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c minals Push-button type Input voltage Input voltage Number of terminals Functions Output type Output voltage Kaximum input voltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2 us or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V). Falling: Triggering occurs. <sup>1</sup> Trigger ining: With the START&STOP option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions <b>External control te</b> Terminal block External input	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Number of terminals Functions Output type Output voltage Kaximum input voltage External trigger filter Response pulse width Functions Output type Output voltage Maximum input voltage Maximum input voltage Width	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2 ms or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 0.8 V) or high (2.5 V to 10 V). Falling: Triggering occurs withs TART&STOP option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level roulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output External output	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c rminals Push-button type Input voltage Input voltage Number of terminals Functions Output type Output voltage Maximum input voltage Karmal trigger filter Response pulse width Functions Output type Output voltage Maximum input voltage Output type Output voltage Maximum input voltage Maximum input voltage Width Functions Output type Output voltage Maximum input voltage Output voltage Maximum input voltage Maximum input voltage Output type Output voltage Output type Output voltage Output type Output voltage Maximum input voltage Output splase Voltage V	a high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2.5 ms or more during low periods Rising. Triggerting curs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V). Falling: Triggering occurs when the voltage rises from high (2.5 V to 10 V) to low (0 V to 0.8 V) or when a terminal short circuit occurs. "Trigger timing: With the START&STOP option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n</b> signals Hz ±1% square waves	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External output External output External trigger Trigger output Output terminal for Output terminal for Output signals Functions	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Input voltage Maximum input volt	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2 us or more during low periods Rising, Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V), Falling: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 10.8 V) or when a terminal short circuit occurs. *Trigger ting: With the START&STOP option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n signals</b> Hz ±1% square waves 3666 100:1 PROBE correction	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output External output Trigger output Output terminal for Output signals Functions Dedicated power s	SMB 10 V DC 2.5 V to 10 V for higl 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Unput voltage Maximum input voltage Maximum input voltage Maximum input voltage External trigger filter Response pulse width Functions Output type Output voltage Maximum input voltage Maximum input voltage Cutput voltage Maximum input voltage Maximum input voltage Maximum input voltage Output voltage Maximum input voltage Maximum input voltage Width Gutput type Output voltage Output voltage Output voltage Output voltage Output voltage Output voltage Maximum input voltage Output type Output type Output soltage Maximum input voltage Output type Output voltage Maximum input voltage Output type Output type Output soltage Maximum input voltage Output type Output soltage Maximum input voltage Output soltage Maximum input voltage Output type Output soltage Maximum input voltage Output soltage Maximum input soltage Output soltage Maximum input soltage Output soltage Maximum input soltage Output soltage Output soltage Maximum input soltage Output soltage Maximum input soltage Output soltage	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter ON: 2.5 ms or more during high periods, 2 us or more during low periods Rising, Triggering occurs when the voltage rises from low (0 V to 0.8 V) to high (2.5 V to 10 V), Falling: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 10.8 V) or when a terminal short circuit occurs. *Trigger ting: With the START&STOP option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n signals</b> Hz ±1% square waves 3666 100:1 PROBE correction	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External output External output External output Trigger output Output signals Functions Dedicated power s Option to be specified to Number of terminals	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Input voltage Maximum input volt	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter OFS: 2.5 ms or more during high periods, 2.5 ms or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 0.8 V) to high (2.5 V to 10 V). Falling: Trigger ing occurs when the voltage falls from high (2.5 V to 10 V) to 0.8 V) or when a terminal short circuit occurs. *Trigger timing: With the START STOP poption, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n signals</b> Hz ±1% square waves 30666 flo0:1 PROBE correction <b>pre current sensor</b>	
Connector Maximum input voltage Maximum input voltage Response pulse width Maximum input frequency. Functions External control te Terminal block External output External output External output External trigger Trigger output Output terminal for Output signals Functions Dedicated power s Option to be specified to Number of terminals Output voltage	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Input voltage Maximum input volt	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter OFF: 2 ms or more during high periods, 2 ms or more during low periods Rising/Italling selection possible Rising: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 10 V) to 0.5 V or low level 50 V DC, 50 mA, 200 mW 2 Trigger ining: With the START&STOP, Option, rising/ falling can be selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible tuevel: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n signals</b> Hz ±1% square waves 3666 100:1 PROBE correction <b>or current sensor</b> (with 25021 PROBE POWER UNIT installed)	
Connector Maximum input voltage Input voltage Response pulse width Maximum input frequency Functions External control te Terminal block External input External output External output Trigger output Output terminal for Output signals Functions Dedicated power s	SMB 10 V DC 2.5 V to 10 V for higt 50 ns or more during 10 MHz External sampling c rminals Push-button type Maximum input voltage Input voltage Input voltage Maximum input volt	g high periods, 50 ns or more during low periods lock input, rising/falling selection possible 10 V DC 2.5 V to 10 V for high level, 0 V to 0.8 V for low level 50 ms or more during high periods, 50 ms or more during low periods 200 ms or greater 2 START, STOP, START/STOP, SAVE, ABORT, event Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW 2 Judgment (PASS), judgment (FAIL), occurrence of errors, busy, trigger standby 10 V DC ON / OFF External trigger filter OFF: 1 ms or more during high periods, 2 us or more during low periods External trigger filter OFS: 5 ms or more during high periods, 2 ms or more during low periods Rising/falling selection possible Rising: Triggering occurs when the voltage falls from high (2.5 V to 10 V) to 0.8 V) to high (2.5 V to 10 V). Falling: Triggering occurs with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 v DC, 50 mA, 200 mW Level or pulse selected for either START or STOP. Open drain output (active low, with 5 V voltage output) 4.0 V to 5.0 V for high level, 0 V to 0.5 V for low level 50 V DC, 50 mA, 200 mW Level or pulse selection possible Level: Sampling period x data number after trigger Pulse: 2 ms ±1 ms <b>n signals</b> Hz ±1% square waves 3066 100:1 PROBE correction <b>or current sensor</b> (with 25021 PROBE poWER UNIT installed)	

Trigger source	When START or ST "Up to 4 analog tri "Up to 4 logic trigg: "Up to 2 analog trigg: When START&STO Analog: Up to 16 cl Logic: Up to 16 pi Real-time waveforr "Up to 2 trigger ty	me waveform processing OP is selected: Up to 32 channels gers can be set for each analog channel. gers can be set for each logic probe. Jers can be set for each real-time waveform processing channel. P is selected: Up to 16 channels / group nannels / group (Up to 2 channels per unit can be selected.) obes / group (Up to 2 channels per unit can be selected.) n processing: Up to 16 calculations / group gers from each group can be set for each logic probe.
	External trigger	
		n is activated if all trigger sources are turned off.
	Level trigger	Triggering occurs when the set level rises (falls).
	Voltage drop	Triggering occurs when peak voltage drops below the set level. (For a 50 Hz / 60 Hz commercial power supply only)
	trigger	*1, *2, *3
	Window trigger	Sets the upper and lower limit for trigger level. Triggering occurs when leaving (OUT) or entering (IN) the area.
	window ingger	*1
	Period trigger	Sets the period reference value and cycle range. Triggering occurs when the rising (falling) reference value period is measured and determined to be outside or within the cycle range.
Analog triggers		*1, *2, *3 Sets the reference value and pulse width (glitch width).
	Glitch trigger	Triggering occurs if the value is below the set pulse width from rising or falling of the reference value. *1, *Not available with MR8990, *3
	Specifying events	Specifying events (1 to 4000) Counts the number of times conditions were fulfilled for each trigger source. Triggering occurs when the set number of times is reached. *Not available when the trigger conditions are set to AND
		*1: Disabled when sampling rate is set to 200 MS/s. *2: Not available with MR8990 or 8970
Logic trigger	Pattern trigger using	*3: Not available with envelope setting
Forcible trigger		iggering can be prioritized over all trigger sources.)
	Recording possible a	t specified measuring intervals (hours, minutes, or seconds)
Interval trigger	The trigger condition Afterwards, the trigg	ns are fulfilled when the measuring process starts. ger conditions are met at the set measuring intervals. OFF, 10, 20, 50, 100, 150, 200, 250, 500, 1000, 2000,
Trigger filter	Normal	5000, 10,000 samples
Level setting resolution	Envelope 1 LSB	OFF, 1 ms, 10 ms
-		lue set in 1% steps available), displaying the recording
Pre-trigger	time for pre-trigger	
Post-trigger		ng the recording time for post-trigger
Trigger priority Trigger mark	ON / OFF Displays trigger mar	ks for the positions where triggers are set.
Trigger timing	START, STOP, STAR	
Waveform monitoring	Displays the wavefo	rm monitor in the trigger standby state. (The display can
display	be turned off.)	
Waveform screen	Waveform display	1 screen, 2 screens, 4 screens, 8 screens, 16 screens
	in chronological	*Displays up to 64 channels per sheet.
Numerical display format	FFT display	*Multiple sheets can be set for the same channel. 1 screen, 2 screens, 4 screens Waveform in chronological order + FFT display
Sheet function	Up to 16 sheets	(1 screen, 2 screens, 4 screens) *The display format can be selected for each sheet.
		are displayed in chronological order in the top part of the
Zoom display		reas the zoomed waveforms are displayed in the bottom part.)
Full screen display		over the entire waveform screen.
	Waveform color Interpolation	Fixed colors (32 colors) Linear
	Variable display	Always ON
	Vernier	Adjustable input waveform
Waveform display		(Adjustment range: 50% to 250% of the input) OFF / ON
	Grid	Wide / Standard / Narrow
	waveform inversion	*Not available with 8967, 8970, and 8973
Enlarge / Reduce	Allows you to adjust	the zoom ratio as necessary by pinching in or out.
Waveform scrolling	,	swiping the screen and scroll back while measuring.
Roll display mode	The drawing start po	latest data by following the measuring process. sition (left or right edge) can be selected. displayed when the overlay function is turned on.
Waveform monitoring function	ON / OFF (The moni	tor can also be displayed in the trigger standby state.)
	1	
		or manual option can be selected.
Overlay		displayed when the overlay function is turned on.
Overlay		displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference.
	*The roll cannot be o	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed.
Cursor	*The roll cannot be of Tracing cursor	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. *Displays potential and potential difference.
	*The roll cannot be of Tracing cursor Horizontal cursor Gauge	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. *Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2
	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range.
Cursor	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location.
	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range.
Cursor	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. *Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 *Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input.
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. *Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. *Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 *Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 100, 50, 20, 105, 22, 1 [Sr]
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500, 200, 100, 50, 20, 1, 05, 2, 1 [S/s] "The speed for real-time waveform processing can be set from 100 MS/s.
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 K, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 h, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 M, 50 K, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 2 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 50 k, 2 k, 10 k, 5 k, 2 k, 1 k 50 k, 2 k, 10 k, 5 k, 2 k, 10 k, 5 k, 2 k, 1 k 50 k, 2 k, 10 k, 5 k, 2 k, 10 k, 5 k, 2 k, 1 k 50 k, 2 k, 10 k, 5 k, 2 k, 10 k, 5 k, 2 k, 1 k 50 k, 2 k, 10 k, 5 k, 2 k, 10 k, 5 k, 2 k, 1 k k, 2 k, 10 k, 2 k, 10 k, 5 k, 2 k, 1 k k, 2 k, 10
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s] "The speed for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 2 M, 1 M
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500, 200, 100 S, 50, 2, 10 K, 5 K, 2 K, 1 k 500, 200, 100 S, 52, 1 [S/s] "The speed for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 2 M, 1 M 500 K, 200 K, 100 K, 50 K, 20 K, 10 K, 5 K, 2 K, 1 k 500, 200, 100 S, 00, 2, 1 [S/s]
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s] The speed for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 20 M, 10 K, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 00, 50, 20, 10, 5, 2, 1 [S/s] Thus Speed for maximum and minimum values "Calculation speed for maximum and minimum values "Oversampling rate: 100 MS/s.
Cursor Event mark	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 K, 100 k, 50 k, 2 k, 1 k, 500 k, 200 k, 100 k, 50 k, 2 k, 1 k, 500 k, 200 h, 100 k, 50 k, 2 k, 1 k, 500 k, 200 h, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 200 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 20 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 20 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 20 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 20 k, 10 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 50 k, 20 k, 10 k, 50 k,
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling. Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200 , 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope	<ul> <li>displayed when the overlay function is turned on.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential, time from trigger, time difference between cursors, and potential difference.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential and potential difference.</li> <li>Up to 8 gauges can be displayed.</li> <li>Segment cursor 1 / Segment cursor 2</li> <li>Specifies the calculation range, saving range, and search range.</li> <li>Tap the screen to jump to the specified location.</li> <li>g the measuring process (up to 1000 marks) or external input terminal for input.</li> <li>200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s]</li> <li>The speed for real-time waveform processing can be set from 100 MS/s.</li> <li>External sampling: Depending on the input signal of the external sampling terminal Up to 10 HHz</li> <li>10 M, 5 M, 20 K, 10 K, 5 K, 2 K, 1 K 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s]</li> <li>The speed for real-time waveform processing can be set from 100 MS/s.</li> <li>External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz</li> <li>10 M, 5 M, 2 M, 1 M</li> <li>500 K, 20 K, 10 K, 5 K, 2 K, 1 K 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s]</li> <li>30, 12, 6, 2, 1 [S/min]</li> <li>*Calculation speed for maximum and minimum values</li> <li>*Oversampling rate: 100 MS/s</li> <li>Maximum available sampling rate</li> <li>[Save destination: SSD] 20 MS/s (2 channels), 10 MS/s (4 channels), 2 MS/s (16 channels), 1 MS/s (3 channels), 2 MS/s (16 channels), 1 MS/s (3 channels), 2 MS/s (16 channels), 1 MS/s</li> </ul>
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal	<ul> <li>displayed when the overlay function is turned on.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential, time from trigger, time difference between cursors, and potential difference.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential and potential difference.</li> <li>Up to 8 gauges can be displayed.</li> <li>Segment cursor 1 / Segment cursor 2</li> <li>Spacilise the calculation range, saving range, and search range.</li> <li>Tap the screen to jump to the specified location.</li> <li>g the measuring process (up to 1000 marks) or external input terminal for input.</li> <li>200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M</li> <li>500 k, 200 k, 100 k, 50 k, 2 k, 1 k, 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s]</li> <li>The speed for real-time waveform processing can be set from 100 MS/s.</li> <li>External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz</li> <li>10 M, 5 M, 20 M, 10 M, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li></ul>
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 10, 50, 20, 10, 5, 2, 1 [S/s] The speed for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 20 M, 10 K, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s] 30, 12, 6, 2, 1 [S/min] "Calculation speed for maximum and minimum values "Oversampling rate: 100 MS/s Maximum available sampling rate [Save destination: SDD 20 MS/s (2 channels), 10 MS/s (4 channels), 50 MS/s (6 channels), 10 MS/s (4 channels), 50 MS/s (6 channels), 10 MS/s (4 channels), 20 MS/s (6 channne
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving *The values in ( ) indicate	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. g the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500, 200, 100, 50, 20, 10, 5, 2, 1 [S/s] The speed for real-time waveform processing can be set from 100 MS/s. External sampling: Depending on the input signal of the external sampling: Depending on the input signal of the external sampling terminal Up to 10 MHz 10 M, 5 M, 20 M, 10 K, 5 k, 2 k, 1 k 500, 200, 00, 50, 20, 0, 5, 2, 1 [S/s] "Calculation speed for maximum and minimum values "Oversampling rate: 100 MS/s Maximum available sampling rate [Save destination: SDJ 00 KS/s (2 channels), 10 MS/s (4 channels), 50 MS/s (8 channels), 2 MS/s (16 channels), 1 MS/s (32 channels), 500 KS/s (64 channels), [Save destination: SDD memory card, USB memory stick, sending via FTP] 5 MS/s (8 channels), 2 MS/s (8 channels), [Save destination: SD memory card, USB memory stick, sending via FTP] 5 MS/s (8 channels), 2 MS/s
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving *The values in ( ) indicate the number of	<ul> <li>displayed when the overlay function is turned on.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential, time from trigger, time difference between cursors, and potential difference.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential and potential difference.</li> <li>Up to 8 gauges can be displayed.</li> <li>Segment cursor 1 / Segment cursor 2</li> <li>"Specifies the calculation range, saving range, and search range.</li> <li>Tap the screen to jump to the specified location.</li> <li>g the measuring process (up to 1000 marks) or external input terminal for input.</li> <li>200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M</li> <li>500 K, 200 A, 100 K, 50 K, 20 K, 10 K, 5 K, 2 K, 1 K</li> <li>500 K, 200 th real-time waveform processing can be set from 100 MS/s.</li> <li>External sampling: Depending on the input signal of the external sampling terminal</li> <li>Up to 10 MHz</li> <li>10 M, 5 M, 2 M, 1 M</li> <li>500 K, 200 K, 100 K, 50 K, 20 K, 10 K, 5 K, 2 K, 1 K</li> <li>500 K, 200 K, 100 K, 50 K, 20 K, 10 K, 5 K, 2 K, 1 K</li> <li>500 K, 200 K, 100 K, 50 K, 20 K, 10 K, 5 K, 2 K, 1 K</li> <li>500 K, 200 L, 10 K, 5 G Channels), 10 M5/S</li> <li>Maximum available sampling rate</li> <li>[Save destination: SSD] 20 MS/s (64 channels), 10 MS/s (4 channels), 5 MS/s (64 channels), 10 MS/s (32 channels), 200 KS/s (64 channels), 500 KS/s (64 cha</li></ul>
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving *The values in ( ) indicate	<ul> <li>displayed when the overlay function is turned on.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential, time from trigger, time difference between cursors, and potential difference.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential and potential difference.</li> <li>Up to 8 gauges can be displayed.</li> <li>Segment cursor 1 / Segment cursor 2</li> <li>"Specifies the calculation range, saving range, and search range.</li> <li>Tap the screen to jump to the specified location.</li> <li>g the measuring process (up to 1000 marks) or external input terminal for input.</li> <li>200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k/s (2 channels), 10 MS/s</li> <li>Maximum available sampling rate</li> <li>[Save destination: SSD] 20 MS/s (2 channels), 10 MS/s (4 channels), 5 MS/s (6 channels), 10 MS/s (3 channels), 200 K/s (64 channels), 10 KS/s (4 channels), 500 K/s (2 channels), 200 K/s (64 channels), 100 K/s (64 channels), 200 K/s (64 channels), 200 K/s (63 channels), 200 K/s (64 c</li></ul>
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving *The values in ( ) indicate the number of	displayed when the overlay function is turned on. Up to 8 cursors can be displayed. "Displays potential, time from trigger, time difference between cursors, and potential difference. Up to 8 cursors can be displayed. "Displays potential and potential difference. Up to 8 gauges can be displayed. Segment cursor 1 / Segment cursor 2 "Specifies the calculation range, saving range, and search range. Tap the screen to jump to the specified location. Ig the measuring process (up to 1000 marks) or external input terminal for input. 200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k 500 k, 200 k, 100 k, 50 k/s (2 channels), 10 MS/s (4 channels), 50 MS/s (6 channels), 10 MS/s (4 channels), 50 K/s (6 channels), 10 MS/s (4 channels), 50 K/s (6 channels), 10 KS/s (4 channels), 50 K/s (6 channels), 10 KS/s (4 channels), 10 K/s (6 channels), 10 KS/s (4 channels), 10 KS/s (6 channels), 10 KS/s (4 channels), 10 KS/s (6 channels), 10 KS/s (4 channels), 10 KS/s (6 channels), 100 KS/s (5 channels), 100
Cursor Event mark Setting screen	*The roll cannot be of Tracing cursor Horizontal cursor Gauge Specifying segments Jump Input available durin Use the start button Normal Envelope For real-time saving *The values in ( ) indicate the number of	<ul> <li>displayed when the overlay function is turned on.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential, time from trigger, time difference between cursors, and potential difference.</li> <li>Up to 8 cursors can be displayed.</li> <li>Displays potential and potential difference.</li> <li>Up to 8 gauges can be displayed.</li> <li>Segment cursor 1 / Segment cursor 2</li> <li>Spacilise the calculation range, saving range, and search range.</li> <li>Tap the screen to jump to the specified location.</li> <li>g the measuring process (up to 1000 marks) or external input terminal for input.</li> <li>200 M, 100 M, 50 M, 20 M, 10 M, 5 M, 2 M, 1 M</li> <li>500 k, 200 k, 100 k, 50 k, 2 k, 1 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 2 k, 1 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 200 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 2 k, 1 k</li> <li>500 k, 20 k, 100 k, 50 k, 20 k, 10 k, 5 k, 6 channels), 10 MS/s (4 channels), 50 k/s (4 channels), 50 k/s (4 channels), 50 k/s (6 channels), 20 k/s (6 channels), 20 k/s (6 channels), 20 k/s (6 ch</li></ul>

		[Built-in presets (8 channels), 2				nannels), 100 M nnels), 1 G (1
	Normal		ding leng			nels), 67108800 5400 (4 channels),
		536870900 (2 *Setting is pos	channels	s), 1073741	800 (1 chan	
						channels), 50 M annels), 500 M (1
	Envelope	channel) [Poir	nt]			nnels), 33554400
			, 671088	00 (8 chani	nels), 13421	7700 (4 channels),
Maximum recording length	-	*Setting is pos Determined ac				space in the save
	*The values in ( ) indic	destination, file	e system	and numb		urement channels
	How channels are defi 1. 2-channel input uni	ned:			iel	
	<ol> <li>2. 3- or 4-channel unit When either or both C</li> </ol>	ts: (U8975/U89	77/U8978	3):		
	When either or both C Any combination of th	CH3/CH4 are us	ed, coun	ts as 1 cha		
	<ol> <li>Real-time waveform</li> <li>*When using any of Mo</li> </ol>	n processing: ea odel U8975, U8	ich opera 977, U89	ation count 78, or MR8	990, or cor	ducting real-time
	waveform processing, the maximum recording length at a sampling r less does not exceed half the length of the values listed above.			rate of 10 MS/s or		
Repeated measurements	Single, repeated, specified number of times *Repeated measurements cann be set and the number of times cannot be specified for real-time saving.					
Waveform monitoring function	Displayed on the ch Conversion ratio and	-		Model / Or	itnut rate /	dB / Bating
Scaling	*Model: Select a mo *Automatic detection a	del to configu	re the se	caling set	tings auto	matically.
Comments	Title comments, channe Channel numbers and ch	l comments				
	Calculation formulas	32 formulas				
	Calculation targets	8971, 8972, L	8974, U8	3975, U89	76, U8977,	68, U8969, 8970 U8978, U8979
Digital filter	Coloulation un data	*The 8973 and 10 M / 1 M / 1				are not applicable 1 [S/s]
- *MR6000-01 only	Calculation update rate	*Up to 8 calc *Up to 16 cal				
(Option to be specified upon order)	Calculation datas	Calculation update rate	10 MS/s	1 MS/s	100 kS/s	10 kS/s or less
	Calculation delay	Calculation delay	6.2 or 6.3 us	5 us	20 us	Calculation update rate period
	Filter types		F/BPF			PF / BPF / BSF),
Saving						
	SD MEMORY CARD USB MEMORY STICK	Z4001 (2 GB Z4006 (16 G		8 (8 GB)		
Save destination	SSD HDD	U8332 SSD U8333 HD U				
	Sending to FTP	PC with a LAN connection				
File format	Sending e-mails FAT, FAT32, NTFS, e	Send files via	e-mail	to specifi	ed addres	S
Filename Pressessing identical	Alphanumeric and J	apanese inpu	t			
Processing identical filenames	Adding a serial num	ber at the beg	jinning t	pefore sav	ving	
	ON / OFF *Automatically saves a measuring proce		ained fo	r the reco	rding leng	th at the end of
Auto saving	*Settings files are no time saving is sele	ot supported.	*This fur	nction is n	ot availab	le when real-
	*When using memory during saving. (Lin	ry segmentation	on, mea: moling r	surement	of the nex	t block can start
	ON / OFF *Saves the waveforr					
Real-time saving	directly to the save of File division		he auto	saving fu	nction is n	ot available.
Deleting and equips	Deletes the files with	n the oldest cr	eation d	ates and	saves data	a when there is
Deleting and saving	no free space left or for auto saving and	real-time savir		at the sav	e destinat	ION. ENADIEU
	Settings data Waveform data	.SET Binary format	(.MEM, .	REC, .FLT	), text form	at (.TXT, .CSV)
Types of saved data	Index Displayed images	Divided savi		), memory	/ segment	
	Numerical calculation results	BMP PNG	JPG			ation (.SEQ)
Saving channels						
earing onallicio	Select a channel fro channels when savi	.CSV, .TXT m all the chan ng waveform o	nels ava lata.			isplayed
Culled data saving	Select a channel fro channels when savii Waveform data (text (from 2 to 1000) before	.CSV, .TXT m all the chan ng waveform of format) is cul ore saving.	nels ava lata. ed acco			isplayed
Culled data saving	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) befor Types of saved data	.CSV, .TXT m all the chan ng waveform of format) is cul ore saving. Division meth	nels ava lata. ed acco	ording to t	he specifi	isplayed ed culling value
Culled data saving File division *Real-time saving and memory segmentation	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef. Types of saved data Binary format Text format	.CSV, .TXT m all the chan ng waveform of format) is cul ore saving. Division meth OFF / Every 161 OFF / Every 60	nels ava data. ed acco nod MB of data 000 poin	ording to t	he specifie MB of data / Every 1,000	isplayed ed culling value Every 64 MB of data
Culled data saving File division *Real-time saving and memory segmentation excluded	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi	.CSV, .TXT m all the chan ng waveform of format) is cul ore saving. Division mett OFF / Every 161 OFF / Every 60 OFF / By the les *Enabled w	nels ava data. ed acco nod MB of data 000 poin calculat rhen nun	ording to t	he specifie MB of data / Every 1,000 er Iculation re	isplayed ed culling value Every 64 MB of data ,000 points of data sults are saved.
Culled data saving File division *Real-time saving and memory segmentation excluded	Select a channel fro channels when savii Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical aculation results New files / Existing fi "Select whether to crea	.CSV, .TXT m all the chan ng waveform o format) is cul ore saving. Division meth OFF / Every 60 OFF / By the les *Enabled w Press the SAV	nels ava data. led acco nod //B of data 000 poin calculat rhen nun dd data to E button	ording to t	he specifie MB of data / Every 1,000 er Iculation re g file when s ia to a save	isplayed ed culling value Every 64 MB of data 0,000 points of data sults are saved. tarting to measure destination, unde
Culled data saving File division "Real-time saving and memory segmentation excluded Specifying files	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi *Select whether to crea Instant saving	.CSV, .TXT m all the chan ng waveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / By the les *Enabled w te a new file or a Press the SAV a filename, an Select the ful	nels ava Jata. ed acco nod MB of data 000 poin calculat rhen nun dd data to E button d with sav I range o	ording to t (Every 32) ts of data / ion numb nerical cal o an existin to save dat ving setting or a spec	he specifie MB of data / Every 1,000 er Iculation re g file when s ia to a save gs that have ific segme	isplayed ed culling value Every 64 MB of data (000 points of data sults are saved. tatring to measure destination, unde been pre-set. n. *Enabled
Culled data saving File division FReal-time asving and memory segmentation excluded Specifying files SAVE button operation	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerial calculation results New files / Existing fi Select whether to crea Instant saving	.CSV, .TXT m all the chan ng waveform o format) is cul Division mett OFF / Every 60 OFF / By the les *Enabled w te a new file or a Press the SAV a filename, and	nels ava Jata. ed acco nod MB of data 000 poin calculat rhen nun dd data to E button d with sav I range o	ording to t (Every 32) ts of data / ion numb nerical cal o an existin to save dat ving setting or a spec	he specifie MB of data / Every 1,000 er Iculation re g file when s ia to a save gs that have ific segme	isplayed ed culling value Every 64 MB of data (000 points of data sults are saved. tatring to measure destination, unde been pre-set. n. *Enabled
Culled data saving File division FReal-time asving and memory segmentation excluded Specifying files SAVE button operation	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results Numerical calculation results New files / Existing fi "Select whether to creat Instant saving Saving range SD MEMORY CARD	.CSV, .TXT m all the char ng waveform of format) is cul ore saving. Division mett OFF / Every 161 OFF / Every 161 OFF / Every 60 OFF / By the les "Enabled vi te a new file or a Press the SAV a filename, and Select the ful only when da Z4001 (2 GB	nels ava data. ed acco nod MB of data 000 poin calculat then nun dd data to E button n d with sav I range o tta is sav	i/Every 32 ts of data / ion numb herical calo an existin to save dat ving setting or a spec ved with ti	he specifie MB of data / Every 1,000 er Iculation re g file when s ia to a save gs that have ific segme	isplayed ed culling value Every 64 MB of data (000 points of data sults are saved. Jatring to measure destination, unde been pre-set. n. *Enabled
Culled data saving File division FReal-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Namerical calculation results New files / Existing fi *Select whether to crea Instant saving Saving range	.CSV, .TXT m all the char ng waveform of format) is cul ore saving. Division mett OFF / Every 161 OFF / Every 161 OFF / Every 60 OFF / By the les "Enabled vi te a new file or a Press the SAV a filename, and Select the ful only when da Z4001 (2 GB	nels ava data. ed acco MB of data 000 poin calculat then nun dd data to E button i d with san than is	/ Every 32 ts of data / ion numb herical cal o an existin to save dat ving setting or a spec ved with tt (8 GB)	he specifie MB of data / Every 1,000 er Iculation re g file when s ia to a save gs that have ific segme	ed culling value Every 64 MB of data 000 points of data sults are saved. darting to measure destination, unde been pre-set.
Culled data saving File division "Real-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi *Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD	.CSV, .TXT m all the charn growselform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / Every 60 OFF / By the les *Enabled v te a new file or a Press the SAV a filename, an Select the ful only when de Z40001 (2 GB Z4006 (16 Gi U8332 SSD L U8333 HD U	nels ava Jata. ed acco MB of data 000 poin calculat then nun dd data to E button 1 d with san I range o tta is san XI z4003 3) JNIT (25	i/ Every 32 is of data / ion numb herical calo o an existin to save data ving setting or a spec ved with ti (8 GB) 6 GB) GB)	MB of data / Every 1,000 er (culation rer g file when s a to a save gs that have fifc segme he SAVE k	isplayed ed culling value Every 64 MB of data ,000 points of data sults are saved. tarting to measure destination, unde destination, unde destination, unde epen pre-set. nt. "Enabled ey.
Culled data saving File division "Real-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s	.CSV, .TXT m all the charn gwaveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / By the les * Tenabled w les * Tenabled w	nels ava Jata. ed acco MB of data 000 poin calculat rhen nun dd data to b with sau d wit	i/Every 32 ts of data / ion numb herical cai o an existin o save dat ving setting or a spec with tt (8 GB) 6 GB) GB) Binary	MB of data / Every 1,000 er culation reg ga to a save as to at have fifc segme he SAVE k	isplayed ed culling value Every 64 MB of data sults are saved. tarting to measure destination, under been pre-set. nt. *Enabled ey.
Culled data saving File division File division Preal-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available without the same start of the same sta	.CSV, TXT m all the char gwaveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / By the les *Enabled we te a new file or a Press the SAV a filename, an Select the ful only when de Z4001 (2 GB Z4006 (16 Gi U8332 SDD U U8333 HD U Waveforr aving (JDX), r th envelope se	nels ava Jata. ed acco MB of data 000 poin calculat rhen nun dd data to b with sau d wit	i/Every 32 ts of data / ion numb herical cai o an existin o save dat ving setting or a spec with tt (8 GB) 6 GB) GB) Binary	MB of data / Every 1,000 er culation reg ga to a save as to at have fifc segme he SAVE k	isplayed ed culling value Every 64 MB of date (000 points of date sults are saved. tarting to measure destination, unde been pre-set. nt. *Enabled ey.
Culled data saving File division File division Preal-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Text format Text format New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s <b>Ons</b> "Not available wi 16 items x Measurer	.CSV, TXT m all the charn gwaveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / By the les *Enabled we te a new file or a Press the SAV a filename, an Select the ful only when de Z4001 (2 GB Z4006 (16 GI U8333 HD U Waveforr taving (JDX), r th envelope se nent channels	nels ava Jata. ed acco MB of data 000 poin calculat rhen nun dd data to b with sau d wit	i/Every 32 ts of data / ion numb herical cai o an existin o save dat ving setting or a spec with tt (8 GB) 6 GB) GB) Binary	MB of data / Every 1,000 er culation reg ga to a save as to at have fifc segme he SAVE k	isplayed ed culling value Every 64 MB of data sults are saved. tarting to measure destination, under been pre-set. nt. *Enabled ey.
Culled data saving File division File division Preal-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available without the same start of the same sta	.CSV, TXT m all the charn gwaveform of format) is cul ore saving. Division mett OFF / Every 161 OFF / Every 161 OFF / Every 60 OFF / By the les *Enabled vite a new file or a Press the SAV only when da Z4001 (2 GB Z4006 (16 GI U8333 HD U Waveforr isaving (.IDX), r th envelope se nent channels d segments Peak to peak val	nels avv lata. eed accc nod M& of data to calculat M& of data to then nun di data to with say 1, Z4003 3) NIT (320 n data normory : titing	i/Every 32 i/Every 32 ts of data / ion numb nerical cala o an existin o save data ving setting or a spec red with ti (8 GB) 6 GB) Binary segmenta	he specifii MB of data / Every 1,000 er culation reg gile when s a to a save gs that have fifc segme he SAVE k s SAVE k r format (.N tion (.SEQ	isplayed ed culling value Every 64 MB of data (000 points of data sults are saved. iatring to measure destination, under been pre-set. nt. *Enabled ey. //EM, .REC)
Culled data saving File division File division Preal-time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Text format Text format New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s <b>Ons</b> "Not available wi 16 items x Measurer	.CSV, .TXT m all the charn gwaveform of format) is cul ore saving. Division mett OFF / Every 161 OFF / Every 161 OFF / Every 60 OFF / By the les *Enabled vite a new file or a Press the SAV a filename, an Select the ful only when da Z4006 (16 Gi U4832 SSD U U4832 SSD U U4833 HD UI Waveforr aving (.IDX), r th envelope se nent channels d segments Peak to peak val level, average v ime('), fall ime	nels ave atata. ed accc hod AB of data 000 point calculat d data to button in calculat d data twith sas with sas with sas atata ), Z4003 3) NUT (252 vitro in d (320 n data nemory ; vitro in d (320 no d (320) no d (3	i / Every 32 i / Every 32 is sof data / ion numb nerical cato o an existin to save dat ving setting or a spec ced with ti (8 GB) GB) Binary segmenta	he specifi MB of data / Every 1,000 er Iculation re g file when s a to a save g file when s a to a save s that have if ic segme he SAVE k s SAVE k r format (.N. tion (.SEQ	isplayed ed culling value Every 64 MB of data isplayed destination, unde been pre-set. nt. "Enabled ey. //EM, .REC)
Culled data saving File division File trime saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations Calculation range	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Text format Text format New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s <b>Ons</b> "Not available wi 16 items x Measurer	.CSV, TXT m all the charn m gwaveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / Every 60 OFF / By the les *Enabled w te a new file or a Press the SAV a filename, an Select the ful only when de Z4006 (16 Gil U8332 SSD U U8333 HD U Waveforr the envelope se nent channels Segments Peak to peak val level, average va level, average va level, average va level, average va me o'', fall time area value, Xr's	nels ave lata. ed accc ood AB of data 000 poin calculat divits acculat divits acc	(k GB) (k	he specifi MB of data / Every 1,000 er Culation re g file when s a to a save g file when s it to a save g file when s to a save s that have fit a sparse fit	isplayed ad culling value Every 64 MB of data sults are saved. tarting to measure destination, unde destination, unde teen pre-set. nt. *Enabled ey. MEM, .REC) high-level, low- ideviation, rise io (*), pulse count, alfifernoc (*), alfifernoc (*), alfifernoc (*), alfifernoc (*),
Culled data saving File division File trime saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations Calculation range	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Text format Text format Numerical calculation results New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available wi 16 items x Measurer Full range / Specified	.CSV, TXT m all the charn ng waveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / Every 60 OFF / Every 60 OFF / By the les *Enabled w te a new file or a Press the SAV a filename, an Select the ful only when de Z4001 (2 GB Z4006 (16 GI U8332 SSD U U8333 HD U Waveforr th envelope see nent channels d segments Peak to peak value, X-Ya time to maximun specified time le value, x-Ya	nels ave nels ave atata. ed accco MB of data 000 point calculat then nun calculat then nun d data te button in d data te button in d with sa d with sa ta sav ta sav y. Z4003 3) NIT (320 n data 3) NIT (320 n data (%), reque, ereory (%), reque, (%), requ	very and the provided a	he specifi MB of data / Every 1,000 er Culation reg ficulation reg file when s a to a save g file when s to a save g file when s to a save fits sequence fits sequence fits sequence format (.N tion (.SEQ inimum value, standard d (?), duty rat notae (?), phase m value, standard m value, standard st width (?), X	isplayed ad culling value Every 64 MB of data ,000 points of data sults are saved. starting to measure destination, unde been pre-set. nt. *Enabled ey. // // // // // // // // // // // // //
Culled data saving File division File trime saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculations Calculation range	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Text format Text format Numerical calculation results New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available wi 16 items x Measurer Full range / Specified Normal	.CSV, TXT m all the charn gwaveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / By the les 'Enabled wite a new file or a Press the SAV a filename, an Select the ful only when da Z4000 (16 Gi U8333 HD U Waveforr aving (JDX), r th envelope se nent channels d segments Deak to pask val level, average w time (1), fall time area value, XY7 time to maximun specified time le value, amplitude Beginning, avera	nels ave lata. nel ave lata. nel accc nel accc nel accc nel accc nel accc nel accc nel accc nel accc nel accc nel acc nel acco	verding to t (/Every 32) is of data // ion numb herical cal o an existin to save dat ving setting or a spec ved with ti (8 GB) 6 GB) GB) Binary segmenta Binary segmenta um value, mr ve (RMS) ve tor other other other imminum width ('), periot time different time d	he specifii MB of data / Every 1,000 er iculation reg g file when sa to a save gs that have he SAVE k g file when se he SAVE k format (.N. tion (.SEQ inimum value lue, standard d ( <sup>0</sup> ), duy rato ce ( <sup>0</sup> ), phase m value, sper m v	isplayed ad culling value Every 64 MB of data (000 points of data sults are saved. tarting to measure destination, under been pre-set. nt. *Enabled ey. MEM, .REC) ) // EMM, .REC) ) // EMM, .REC) ) // EMM, .REC) ) // EMM, .REC) ) // EMM, .REC) )
Culled data saving File division File division File division excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculation range Calculation items	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi 'Select whether to creat Instant saving Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s ons 'Not available w 16 items x Measurer Full range / Specified Normal	.CSV, TXT m all the charn gwaveform of format) is cul ore saving. DFF / Every 161 OFF / Every	nels ave nels ave ata. ed accc od MB of data accollent ata. data for acalculat data for acalculat data for acalculat data for acalculat data for acalculat data for a	very set of the termination of termination	he specifi MB of data / Every 1,000 er Culation reg file when s a to a save g file when s to a save g file when s to a save if the sequence in the save k r format (.N tion (.SEQ inimum value, standar other (.) phase m value, spectrum the 'statistical m, waveform m, waveform m, mets, real	isplayed ed culling value Every 64 MB of data (000 points of data sults are saved. dastination, unde been pre-set. nt. *Enabled ey. MEM, .REC) ) high-level, low- devation, rise io (*), pulse count, alfiferince (*), ilidel avel time, perations, median processing results - time waveform
Culled data saving	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi *Select whether to creat Instant saving Saving range Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD Settings data (SET) Index Divided s Ons "Not available wi 16 items x Measurer Full range / Specified Normal	.CSV, TXT m all the charn ng waveform of format) is cul ore saving. Division mett OFF / Every 60 OFF / Every 60 OFF / Every 60 OFF / By the les *Enabled w te a new file or a Press the SAV a filename, an Select the ful only when de Z4006 (16 Gil U8332 SSD U U8333 HD UI Waveforr U8333 HD UI Waveforr the envelope se nent channels Segments Peak to peak vallevel, average w level, average w avalue, Xr5 Peak to peak vallevel, average welvel, average w value, amplitude overshoot, unde Beginning, avera Analog char	nels ave lata. ed accco vod JB of data 000 poin data to data to data to data to data to acalculat then nun dd data to acalculat then nun dd data to acalculat then nun dd data to acalculat then nun dd data to acalculat then nun dd data then nun dd then nun dd data then nun dd then nun dd	urr value, mr view (RMS) value, bur view (RMS) value, bur value, b	he specifi MB of data / Every 1,000 er Culation reg file when s a to a save g file when s to a save g file when s to a save if the sequence in the save k r format (.N tion (.SEQ inimum value, standar other (.) phase m value, spectrum the 'statistical m, waveform m, waveform m, mets, real	isplayed ad culling value Every 64 MB of data (000 points of data sults are saved. dastination, undel been pre-set. nt. *Enabled ey. MEM, .REC) ) Atem, rise io (*), pulse count, afference (*), ifield evel time, perators, median processing results - time waveform
Culled data saving File division File division File division Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical judgment Waveform processin	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available wi 16 items x Measurer Full range / Specified Normal Targeted waveforms Judgment settings Stop conditions	.CSV, TXT m all the charn ng waveform of format) is cul ore saving. Division mett OFF / Every 16 I OFF / Eve	nels ave lata. ed accc MB of data 000 point calculat calculat d with sai d with sai d with sai d with sai sai ta is sai 3) NIT (320 n data 3) NIT (320 n data sis, 74003 3) NIT (320 NIT (320 NI	um value, m via (RMS) via	he specifi MB of data / Every 1,000 er Iculation reg g file when s a to a save g file when s a to a save g file when s have he SAVE k format (.N. tion (.SEQ inimum value lue, standard d (?), duty rat ve (?), phase m value, speer arithmetic og t width (?), X th "Statistical m, waveform nels, real n processi	isplayed ad culling value Every 64 MB of data (000 points of data sults are saved. sults are saved. tarting to measure destination, unde been pre-set. nt. *Enabled ey. MEM, .REC) ) , high-level, low- deviation, rise io (*), puse count, deviation,
Culled data saving File division File time saving and memory segmentation excluded Specifying files SAVE button operation Loading data Loading source Types of loaded data Numerical calculati Maximum number of calculation range Calculation items	Select a channel fro channels when savi Waveform data (text (from 2 to 1000) bef Types of saved data Binary format Text format Numerical calculation results New files / Existing fi Select whether to crea Instant saving Saving range SD MEMORY CARD USB MEMORY CARD USB MEMORY STICK SSD HDD Settings data (.SET) Index Divided s Ons "Not available wi 16 items x Measurer Full range / Specified Normal Targeted waveforms Judgment settings Stop conditions	.CSV, TXT mall the charn ng waveform of format) is cul ore saving. Division mett OFF / Every 16 I OFF / Ever	nels ave lata. ed accc MB of data 000 point calculat calculat d with sai d with sai d with sai d with sai sai ta is sai 3) NIT (320 n data 3) NIT (320 n data sis, 74003 3) NIT (320 NIT (320 NI	um value, m via (RMS) via	he specifi MB of data / Every 1,000 er Iculation reg g file when s a to a save g file when s a to a save g file when s have he SAVE k format (.N. tion (.SEQ inimum value lue, standard d (?), duty rat ve (?), phase m value, speer arithmetic og t width (?), X th "Statistical m, waveform nels, real n processi	isplayed ad culling value Every 64 MB of data ,000 points of data sults are saved. sults are saved. tarting to measure destination, under been pre-set. nt. *Enabled ey. MEM, .REC) ) , high-level, low- deviation, rise io (?), puse count, adifference (?). Sified level time, poreations, median Y waveform angle, function available for y waveform angle, function available for processing results

Maximum recording length	2,000,000 points				
Standard operator	+, -, ×, ÷ Absolute value, exponen	tiation common l	narithe	ioving and	ane derivative integral
Calculation items	secondary derivative, see COS, TAN, ASIN, ACOS, average value (*), maxim *The calculation resu	condary integral, s , ATAN, ATAN2, Fl ium value (*), mini ults can be use	square root IR (LPF, HF mum value ed as the	, cube root PF, BPF, BS (*), level a constant	t, parallel move, PLC shift, SIN, SF), IIR (LPF, HPF, BPF, BSF), t specified time (*) t in the equation.
Averaging function	2 to 10,000 times) *Roll display not availa *One simple averaging	ble when the av	eraging fu three calc	inction is ulation sp	setting for rotations from turned on. ots. (The two calculations averaging will be unavailable.)
Real-time waveform	1	Option to be spe	cified upo	on order (	Order code: MR6000-01)
Maximum number of calculations Calculation targets	U8974, MR8990 (*).	U8975, U8976	. U8977.	U8978.	, 8970, 8971, 8972, 8973, U8979
Calculation update	10 M, 1 M, 100 k, 10	) k, 1 k, 100, 10	D, 1 [S/s]		6 bits of the 24-bit AD resolution.
rate	cannot be set with c	ertain calculati	on updat		
Calculation delay	selected for calculation	6.2 or 6.3 us isted below whe on. 10 MS/s	5 us en real-tim 1 MS/s	20 us le wavefo 100 kS/s	10 kS/s or less Calculation update rate period rm processing channels are 10 kS/s or less
Calculation type					Calculation update rate period erations with coefficients, quartic erentiation, integrals, integration,
	FIR (LPF / HPF / BPF / BS	SF), IIR (LPF / HPF	/ BPF / BS	SF), moving	average, delay device eously with real-time saving
Maximum number of calculations		pe setting, not	available	Simultan	eously with real-time saving
Frequency range	500 mHz to 100 MHz	z (sampling rat	e x0.5), e	external s	sampling
Number of sampling points	1 k, 2 k, 5 k, 10 k, 20	0 k, 50 k, 100 k			
Frequency resolution	1/500, 1/1000, 1/250				
Anti-aliasing filter	AAF (8968, U8979), waveform processin			.PF filter	(FIH, IIH), real-time
Calculation targets				real-time v	vaveform processing results
Analyzed data	Newly loaded				sing START key
	Memory				or data loaded from media
FFT analysis mode setting					CH phase spectrum, cross n, 2CH phase spectrum
Windows	Rectangular, Hanning	, Hamming, Bla			Harris, Flat-top, Exponential
Display scale	Linear scale, log sca				
Peak value display	OFF, local maxima, i Simple averaging, e			eak hold	(arbitrary setting from
Averaging function	2 to 10,000 times)				Carolinary Setting 1011
Calculation execution button	Execution button dis	played in scre	en		
Memory division Max. divisions	1024 blocks				
Block search	Search from the data	a that is saved	in divide	d memo	v block.
Bulk save	Saves entire range of				
Waveform search					
Search mode	Trigger Peak CONCIERGE	selected as th *Logic trigger Maximum valu Histogram, st *Select wheth waveform or t *Disabled wit	search is search is search is andard c her to cor to the diru h envelop	a available ed chann s not avai um value, leviation npare ea ectly pre pe setting	lable with envelope setting. local maxima, local minima ch value to the reference ceding waveform.
	Jump Full range		ne numbe	r of points	e time, relative time, or time s), trigger point, search mark ernal memory
Search range	Specifying segments	Select either the specified for the specified fo			ed for segment 1 or the one
Number of searches	Specifiable (Up to 1)			L	
Continuous search		d number, the			hits in the search range llowing the last search
Display method Other	Specify a search loc	ation to displa	y the dat	a.	
Auto setup	Available previously *The HDD	power is turne saved (START /SSD, SD mem for the save lo	UP.SET) ory card,	to start unit load	ds the settings data up. B memory are searched, in
Rotary knobs	display po	sition can be c	changed	and the o	te, compression rate, or cursor can be moved.
	or display	position can b	e change		range, compression rate, le cursor can be moved.
Shortcut button		can be allocat			ank you go for the state
Auto range	waveform are autom *Not available for en	atically set.) velope, real-tir	ne saving	g, or exte	
Key lock	Three levels of settin and hard buttons.	ys are available	e: UFF, to	ouch scre	een only, or touch screen
Beep sound	OFF / Alarm only / A		ation		
	Sending e-mails via				he CAVE have
Sending e-mails	Sending timing				the SAVE button ain text or files specified by
	Sent data	a type of save	ed data.		
Initialization	Waveform data initia		-		nplete initialization
Self-check Language	Memory, LCD, butto English, Japanese	ns, LAN, media	a, touch s	screen	
Error and warning display	Displays the details	of errors and w	varninas	when the	y occur.
Touch keyboard	Displays the on-scre				·
Region specifications	(text) files and nume Decimal point	rical calculatio Period, comm	in result f na	iles	ata saved to waveform
Time value display	Break Hours, sexagesimal	Comma, space time, date, date		GUICOIOL	1
Zero position display	ON / OFF	,, util			
Waveform screen	Black or white				
background color		*Permitted: If ant	tinge are o	hannod d	iring the measuring process, the
Restart permission					uring the measuring process, the
Disates a state as	diffe to rootdi todi. Hot poi				
Display settings	Adjust brightness or		y to turn o	off autom	
Time settings	Adjust brightness or Set the date and tim		y to turn o	off autom	
	Adjust brightness or Set the date and tim ON / OFF Protects the system recommend turning	e. against uninter off the system	ntional po	ower shu	tdowns. (However, we n and mounting an
Time settings System protection	Adjust brightness or Set the date and tim ON / OFF Protects the system recommend turning external UPS when u	e. against uninter off the system using the unit c	ntional po protectic	ower shu in functic sly for lo	tdowns. (However, we n and mounting an
Time settings System protection function Number of current sensor connections	Adjust brightness or Set the date and tim ON / OFF Protects the system recommend turning external UPS when u Up to 9 connections UNIT 8971, and 3ch	e. against uninter off the system using the unit c altogether on CURRENT UN	ntional po protectic ontinuou the PROE	ower shu in functic sly for lo BE POW	tdowns. (However, we n and mounting an ng periods of time.)
Time settings System protection function Number of current	Adjust brightness or Set the date and tim ON / OFF Protects the system recommend turning external UPS when u Up to 9 connections	e. against uninter off the system using the unit c altogether on CURRENT UN 71: Up to 4 slot:	ntional po protectic ontinuou the PROI IIT U897 s	ower shu in functic sly for lo BE POW	tdowns. (However, we n and mounting an ng periods of time.)

## **Option Specifications** (sold separately)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 280 g (9.9 oz)

Accessories: Noi	ne	
HIGH SPEED ANAL U8976	.OG UNIT	(Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm-up time and zero adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2,	or voltage measurement
Input terminals	Max. rated voltage t the maximum voltage	actor (input impedance 1 $M\Omega$ , input capacitance 22 pF) o ground:1000 V AC, DC (with input isolated from the unit, le that can be applied between input channel and chassis channels without damage)
Measurement range		00, 200, 400 V f.s., 12 ranges ible measurement/display: 280 V rms
Measurement resolution	1/1600 of measuren	nent range (using 12-bit A/D conversion)
Maximum sampling rate	200 MS/s (simultane	eous sampling in 2 channels)
Measurement accuracy	±0.5% f.s. (with filte	r 5 Hz, zero position accuracy included)
Frequency characteristics	DC to 30 MHz -3 dE	8 (with AC coupling: 7 Hz to 30 MHz -3 dB)
Input coupling	AC/DC/GND	
Maximum input	400 V DC (with dire	ct input), 1000 V DC (with 9665)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None

ANALOG UNIT 896	(Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% FH after 30 minutes of warm- up time and zero adjustment; Accuracy guaranteed for 1 year, Post- adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for voltage measurement
Input terminals	Isolated BNC connector (input impedance 1 MΩ, input capacitance 30 pF), Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	100, 200, 400 mV f.s. 1, 2, 4, 10, 20, 40, 100, 200, 400 V f.s., 12 ranges AC voltage for possible measurement/display: 280 V rms Low-pass filter: 5/50/500/5 k/50 k/500 kHz
Measurement resolution	1/2000 of measurement range (using 12-bit A/D conversion)
Maximum sampling rate	20 MS/s (simultaneous sampling across 2 channels)
Measurement accuracy	±0.5% f.s. (with filter 5 Hz, zero position accuracy included)
Frequency characteristics	DC to 5 MHz -3 dB (with AC coupling: 7 Hz to 5 MHz -3 dB)
Input coupling	AC/DC/GND
Maximum input voltage	400 V DC (the maximum voltage that can be applied across input pins without damage)

Accessories. No	ine in the second se
HIGH RESOLUTIO 8968	N UNIT (Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm-up time and zero adjustment; Accuracy guaranteed for 1 yea Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for voltage measurement
Input terminals	Isolated BNC connector (input impedance 1 MΩ, input capacitance 30 pF), Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	100, 200, 400 mV f.s. 1, 2, 4, 10, 20, 40, 100, 200, 400 V f.s., 12 ranges AC voltage for possible measurement/display: 280 V rms Low-pass filter: 5/50/500/5 k/50 kHz
Anti-aliasing filter	Integrated filter for suppressing aliasing distortion caused by FFT processing (automatic cutoff frequency setting/OFF)
Measurement resolution	1/32,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	1 MS/s (simultaneous sampling across 2 channels)
Measurement accuracy	±0.3% f.s. (with filter 5 Hz, zero position accuracy included)
Frequency characteristics	DC to 100 kHz -3 dB (with AC coupling: 7 Hz to 100 kHz -3 dB)
Input coupling	AC/DC/GND
Maximum input voltage	400 V DC (the maximum voltage that can be applied across input pins without damage)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None



0 0

DC/RMS UNIT 897	2 warm-up time and zero adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for voltage measurement, DC/RMS selectable
Input terminals	Isolated BNC connector (input impedance 1 $M\Omega$ , input capacitance 30 pF). Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	100, 200, 400 mV f.s. 1, 2, 4, 10, 20, 40, 100, 200, 400 V f.s., 12 ranges AC voltage for possible measurement/display: 280 V rms Low-pass filter: 5/50/500/5 k/100 kHz
Measurement resolution	1/2000 of measurement range (using 12-bit A/D conversion)
Maximum sampling rate	1 MS/s (simultaneous sampling across 2 channels)
Measurement accuracy	±0.5% f.s. (with filter 5 Hz, zero position accuracy included)
RMS measurement	RMS accuracy: ±1% f.s. (DC, 30 Hz to 1 kHz) ±3% f.s. (1 kHz to 100 kHz) Response time: SLOW 5 s (rise time from 0 to 90% of full scale), MID 800 ms (rise time from 0 to 90% of full scale), FAST 100 ms (rise time from 0 to 90% of full scale) Crest factor: 2
Frequency characteristics	DC to 400 kHz -3 dB (with AC coupling: 7 Hz to 400 kHz -3 dB)
Input coupling	AC/DC/GND
Maximum input voltage	400 V DC (the maximum voltage that can be applied across input pins without damage)

# Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None



0000

6-6

4CH ANALOG UNI	T U8975 (Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm-up time and zero adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 4, for voltage measurement
Input terminals	Isolated BNC connector (input impedance 1 $M\Omega$ , input capacitance 30 pF), Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)
Measurement range	4, 10, 20, 40, 100, 200 V f.s., 6 ranges AC voltage for possible measurement/display: 140 V rms Low-pass filter: 5/500/5 k/200 kHz
Measurement resolution	1/32,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	5 MS/s (simultaneous sampling in 4 channels)
Measurement accuracy	$\pm 0.1\%$ f.s. (with filter 5 Hz, zero position accuracy included)
Frequency characteristics	DC to 2 MHz -3 dB
Input coupling	DC / GND
Maximum input voltage	200 V DC (the maximum voltage that can be applied across input pins without damage)

(Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minute warm-up time and zero adjustment; Accuracy guaranteed for Post-adjustment accuracy guaranteed for 1 year) U8974 No. of channels: 2, for voltage measurement, DC/RMS selectable Max. rated voltage to ground: 1000 V AC, DC for measurement category III, 600 V AC, DC for measurement category IV Measurement functions

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 230 g (8.1 oz) Accessories: None

HIGH-VOLTAGE UNIT

Input terminals	Banana input terminal (Input impedance: 4 MΩ, Input capacitance: 5 pF)
Measurement range	4, 10, 20, 40, 100, 200, 400, 1000 V f.s. (DC mode), 8 ranges 10, 20, 40, 100, 200, 400, 1000 V f.s. (RNS mode), 7 ranges Low-pass filter: 5/50/500/5 k/50 kHz
Measurement resolution	1/32,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	1 MS/s
Measurement accuracy	±0.25% f.s. (with filter 5 Hz, zero position accuracy included)
RMS measurement	RMS accuracy: ±1.5% f.s. (DC, 30 Hz to 1 kHz), ±3% f.s. (1 kHz to 100 kHz) Response time: High speed 150 ms, medium speed 500 ms, low speed 2.5 s
Frequency characteristics	DC to 100 kHz -3 dB
Input coupling	DC / GND
Maximum input voltage	1000 V DC, 700 V AC

Dimensions/mass: approx. 106 mm (4.17 in) W  $\times$  19.8 mm (0.78 in) H  $\times$  196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None

4CH ANALOG UNI	T U8978 (Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm-up time and zero adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 4, for voltage measurement
Input terminals	Isolated BNC connector (input impedance 1 M $\Omega$ , input capacitance 30 pF), Max. rated voltage to ground: 30 V AC or 60V DC for direct input, 300 V AC, DC (CAT II) when combined with the 9665 (Between each input channel and the main unit, and between the input channels)
Measurement range	100, 200, 400 mV f.s. 1, 2, 4, 10, 20, 40 V f.s. 9 ranges Low-pass filter: 5/500/5 k/200 kHz
Measurement resolution	1/32,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	5 MS/s (simultaneous sampling in 4 channels)
Measurement accuracy	±0.3% f.s. (with filter 5 Hz, zero position accuracy included)
Frequency characteristics	DC to 2 MHz -3 dB
Input coupling	DC / GND
Maximum input voltage	40 V DC (with direct input), 400 V DC (with 9665)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 260 g (9.2 oz)

DIGITAL VOLTMET MR8990	FER UNIT (Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm-up time and calibration, Accuracy guaranteed for 1 year, Post- adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for DC voltage measurement
Input terminals	Banana input connectors (Input resistance: 100 M $\Omega$ or higher with 100 mV f.s. to 10 V f.s. range, otherwise 10 M $\Omega$ ) Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channel without damage)
Measurement range	100, 1000 mV f.s. 10, 100, 1000 V f.s., 5 ranges
Measurement resolution	1/1,000,000 of measurement range (using 24-bit $\Delta\Sigma$ modulation A/D)
Integration Time	20 ms × NPLC (during 50 Hz), 16.67 ms × NPLC (during 60 Hz)
Response time	2 ms +2× integration time or less (rise - f.s. $\rightarrow$ + f.s., fall + f.s. $\rightarrow$ - f.s.)
Basic measurement accuracy	±0.01% rdg. ±0.0025% f.s. (at range of 1000 mV f.s.)
Maximum input voltage	500 V DC (the maximum voltage that can be applied across input pins without damage)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 245 g (8.6 oz) Accessories: CONVERSION CABLE L9769 x 2 (cable length 60 cm (1.97 ft))

(Accuracy at 23 ±5°C/73 ±9°F, 80% RH or less a warm-up time and auto-balance: Accuracy quar **STRAIN UNIT U8969** 1 year, Post-adjustment accuracy guarantee d for 1 y No. of channels: 2, for distortion measurement (electronic auto-balancing, Measurement functions balance adjustment range within ±10,000 µc or less) NDIS connector EPRC07-R9FNDIS (via CONVERSION CABLE L9769, NDIS connector PRC03-12A10-7M10.5) Input terminals Max. rated voltage to ground: 30 V AC rms or 60 V DC (with input isolated from the main unit, the maximum voltage that can be applied between input channel and chassis, and between input channels without damage) Strain gauge converter, Suitable transducer Bridge impedance:  $120 \Omega$  to  $1 k\Omega$ , Bridge voltage:  $2 V \pm 0.05 V$ , Gauge rate: 2.0 400, 1000, 2000, 4000, 10,000, 20,000 με f.s., 6 ranges Measurement range Low-pass filter: 5/10/100/1 kHz Measurement resolution 1/25,000 of measurement range (using 16-bit A/D conversion) Maximum sampling rate 200 kS/s (simultaneous sampling across 2 channels) Measurement accuracy ±0.5% f.s. ±4 με (5 Hz filter ON) After auto-balancing Frequency DC to 20 kHz +1/-3 dB characteristics

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 230 g (8.1 oz) Accessories: None

Accessories. N	lone
CHARGE UNIT U897	(Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% RH after 30 minutes of warm- up time and zero adjustment, Accuracy guaranteed for 1 year, Post- adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for acceleration measurement
Input terminals	Voltage input / pre-amp embedded input: Metal BNC connector (Under voltage input: input impedance 1 MΩ, input capacitance 200 pF or less) Charge input: Miniature connector (#10-32UNF) Max. rated voltage to ground: 30 V AC or 60 V DC (with input isolated from the main unit, the maximum voltage that can be applied between input channel and chassis, and between input channels without damage) *Voltage input terminal GND and charge input terminal GND for the same channel are shared.
Suitable transducer	Charge output type acceleration detector Pre-amp embedded acceleration detector
Measurement range Charge input (Miniature connector) Pre-amp embedded input (BNC connector)	1 (m/s <sup>2</sup> ) to 200 k (m/s <sup>2</sup> ) f.s., 12 ranges x 6 types Charge input sensitivity: 0.1 to 10 pC /(m/s <sup>2</sup> ) Pre-amp embedded sensor input sensitivity: 0.1 to 10 mV /(m/s <sup>2</sup> ) Amplitude accuracy: ±2% f.s. Frequency characteristics: 1(1.5) to 50 kHz -3 dB (charge input) Low-pass filter: 500/5 kHz Pre-amp supply power: 3.5 mA ±20%. 22 V ±5% Maximum input charge: ±500 pC (6 ranges on high sensitivity side), 50.000 pC (6 ranges on low sensitivity side)
Measurement range Voltage input (BNC connector)	10 mV to 40 V f.s., 12 ranges, DC amplitude accuracy: ±0.5% f.s. Frequency characteristics: DC to 50 kHz -3 dB (with DC coupling), 1 Hz to 50 kHz -3 dB (with AC coupling) Low-pass filter: 5/500/5 kHz, input coupling: AC/DC/GND Maximum input voltage: 40 V DC
Measurement resolution	1/25,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	200 kS/s
Anti-aliasing filter	Integrated filter for suppressing aliasing distortion caused by FFT processing (automatic cutoff frequency setting/OFF)
TEDS	IEEE 1451.1.4 class 1 support (Support for sensor information reading and automatic sensitivity setting)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: CONVERSION CABLE 9318 x 2 (To connect the current sensor to the 8971)

CURRENT UNIT 897	(Accuracy at 23 ±5°C/73 ±9°F, 20 to 80% FH after 30 minutes of warm- up time and zero adjustment; Accuracy guaranteed for 1 year, Post- adjustment accuracy guaranteed for 1 year)	
Measurement functions	No. of channels: 2, Current measurement with optional current sensor	
Input terminals	Sensor connector (input impedance 1 M $\Omega$ , exclusive connector for current sensor via conversion cable the 9318, common GND with recorder)	
Compatible current sensors	CT6862, CT6863, 9709, CT6865, CT6841, CT6843, CT6844, CT6845, CT6846, 9272-10 (To connect to the 8971 via the CONVERSION CABLE 9318)	
Measurement range	Using 9272-10 (20 A), CT6841: 2 A to 100 A f.s., 6 ranges Using CT6862: 4 A to 200 A f.s., 6 ranges Using 9272-10 (200 A), CT6843, CT6863: 20 A to 1000 A f.s., 6 ranges Using CT6844, CT6845, 9709, CT6846*1, CT6865*1: 40 A to 2000 A f.s., 6 ranges *1: The conversion ratio needs to be set to 2 for scaling.	
Measurement accuracy (with 5 Hz filter ON)	±0.65% f.s. RMS accuracy: ±1% f.s. (DC, 30 Hz to 1 kHz), ±3% f.s. (1 kHz to 10 kHz)	
Note: Add the accuracy and attributes of the current sensor being used.	RMS response time: 100 ms (rise time from 0 to 90% of full scale) Crest factor: 2 Frequency characteristics: DC to 100 kHz ±3 dB (with AC coupling: 7 Hz to 100 kHz)	
Measurement resolution	1/2000 of measurement range (using 12-bit A/D conversion)	
Maximum sampling rate	1 MS/s (simultaneous sampling across 2 channels)	
Other functions	Input coupling: AC/DC/GND, Low-pass filter: 5/50/500/5 k/50 kHz	

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 190 g (6.7 oz) Accessories: None



Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None

. 0 0

....





Measurement functions	No. of channels: 3, Current measurement with optional current sensor
Input terminals	Dedicated connector terminal (ME15W) (input impedance 1 M $\Omega$ , common GND with recorder)
Compatible current sensors	9272-05, CT6841-05, CT6843-05, CT6844-05, CT6845-05, CT6846-05, CT6862-05, CT6863-05, 9709-05, CT6904, CT6865-05, CT6875, CT6876 (Direct connection) CT7631, CT7636, CT7642, CT7731, CT7736, CT7742, CT7044, CT7045, CT7046 (Connection using optional CONVERSION CABLE CT9920)
Measurement range	<ul> <li>Directly connected current sensor: Automatically identify rating of compatible current sensors</li> <li>Using 9272-05 (20 A), CT6841-05: 2 A to 100 A f.s., 6 ranges</li> <li>Using CT6862-05: 4 A to 200 A f.s., 6 ranges</li> <li>Using CT6862-05: 4 A to 200 A f.s., 6 ranges</li> <li>Using CT6844-05, CT6845-05, CT6863-05: 20 A to 1000 A f.s., 6 ranges</li> <li>Using CT6844-05, CT6845-05, CT6904, CT6875: 40 A to 2000 A f.s., 6 ranges</li> <li>Using CT6846-05, CT6845-05, CT6876: 80 A to 4000 A f.s., 6 ranges</li> <li>Using CT6846-05, CT6865-05, CT6876: 80 A to 4000 A f.s., 6 ranges</li> <li>Using CT631, CT7731: 200 A, 1 range</li> <li>Using CT7634, CT7742: 2000 A /1000 A, 3 ranges</li> <li>Using CT7044, CT7045, CT7046: 2000 A to 10,000 A, 3 ranges</li> </ul>
Measurement accuracy (with 5 Hz filter ON) Note: Add the accuracy and attributes of the current sensor being used.	±0.3% f.s. Frequency characteristics: DC to 2 MHz ±3 dB
Measurement resolution	1/32,000 of measurement range (using 16-bit A/D conversion)
Maximum sampling rate	5 MS/s (simultaneous sampling in 3 channels)
ther functions Input coupling: DC/GND, Low-pass filter: 5/500/5 k/200 kHz	
	s: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) 05 in) D, approx. 240 g (8.5 oz) tire clamp x 2

TEMP UNIT 8967	adjustment; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year)
Measurement functions	No. of channels: 2, for temperature measurement with thermocouple (voltage measurement not available)
Input terminals	Thermocouple input: Push-button terminal block, Recommended wire diameter: single-wire 0.14 to 1.5 mm <sup>2</sup> , braided wire 0.14 to 1.0 mm <sup>2</sup> (conductor wire diameter $\phi$ 0.18 mm (0.01 in) or more), AWG 26 to 16 lnput impedance: min. 5 MΩ (with line fault detection ON/OFF) Max. rated voltage to ground: 300 V AC, DC (with input isolated from the unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage)
Temperature measurement range Note: Upper and lower limit values depend on the thermocouple	200°C (392°F) f.s. (-100°C to 200°C (-148°F to 392°F)), 1000°C (1832°F) f.s. (-200°C to 1000°C (-328°F to 1832°F)), 2000°C (3632°F) f.s. (-200°C to 2000°C (-328°F to 3632°F)), 3 ranges Measurement resolution: 1/20,000 of measurement range (using 16-bit A/D conversion)
Thermocouple range (JIS C 1602-1995) (ASTM E-988-96)	K: -200°C to 1350°C (-328°F to 2462°F), J: -200°C to 1100°C (-328°F to 2012°F), E: -200°C to 800°C (-328°F to 1472°F), T: -200°C to 400°C (-328°F to 752°F), N: -200°C to 1300°C (-328°F to 2372°F), N: 0°C to 1700°C (32°F to 3092°F), S: 0°C to 1700°C (32°F to 3092°F), B: 400°C to 1800°C (752°F to 3272°F), W (WRe5-26): 0 to 2000°C (32°F to 3632°F) Reference junction compensation: internal/ external (switchable), line fault detection ON/OFF possible
Data refresh rate	3 methods, Fast:1.2 ms (digital filter OFF), Normal:100 ms (digital filter 50/60 Hz), Slow: 500 ms (digital filter 10 Hz)
Measurement accuracy	Thermocouple K, J, E, T, N: $\pm 0.1\%$ f.s. $\pm 1^{\circ}C$ ( $\pm 1.8^{\circ}F$ ), ( $\pm 0.1\%$ f.s. $\pm 2^{\circ}C$ ( $\pm 3.6^{\circ}F$ ) at $\pm 200^{\circ}C$ to $0^{\circ}C$ ( $-328^{\circ}F$ to $32^{\circ}F$ )) Thermocouple R, S, B, W: $\pm 0.1\%$ f.s. $\pm 3.5^{\circ}C$ ( $\pm 6.3^{\circ}F$ )(at $0^{\circ}C$ ( $32^{\circ}F$ ) to less than $400^{\circ}C$ ( $752^{\circ}F$ ); However, no accuracy guarantee at less than $400^{\circ}C$ ( $752^{\circ}F$ ) for B), $\pm 0.1\%$ f.s. $\pm 3^{\circ}C$ ( $\pm 5.4^{\circ}F$ ) (at $400^{\circ}C$ or more) Reference junction compensation [RJC] accuracy: $\pm 1.5^{\circ}C$ ( $\pm 2.7^{\circ}F$ ) (added to measurement accuracy with internal reference junction compensation)

Dimensions/mass: approx. 106 mm (4.17 in) W x 19.8 mm (0.78 in) H x 196.5 mm (7.74 in) D, approx. 250 g (8.8 oz) Accessories: None 0 0 (Accuracy at 23  $\pm5^\circ\text{C/73}$   $\pm9^\circ\text{F}$  20 to 80 % RH after 30 minutes of warm-up time; Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year) FREQ UNIT 8970 No. of channels: 2, for voltage input based frequency measurement, Measurement Isolated BNC connector (input impedance 1 M $\Omega$ , input capacitance 30 pF), Isolated BNC connector (input impedance 1 M $\Omega$ , input capacitance 30 pF), functions Max. rated voltage to ground: 300 V AC, DC (with input isolated from the Input terminals unit, the maximum voltage that can be applied between input channel and chassis and between input channels without damage) Measurement range: Between DC to 100 kHz (minimum pulse width 2 µs), 20 Hz to 100 kHz f.s., 8 ranges Accuracy: ±0.1% f.s. (exclude 100 kHz range), ±0.7% f.s. (100 kHz range) Frequency mode Measurement range: Between 0 to 2 million rotations/minute (minimum pulse width 2 µs), 2 kr/min to 2 Mr/min f.s, 7 ranges Rotation mode Accuracy: ±0.1% f.s. (exclude 2 Mr/min range), ±0.7% f.s. (2 Mr/min range) Measurement range: 50 Hz (40 to 60 Hz), 60 Hz (50 to 70 Hz), 400 Hz (390 to Power frequency 410 Hz), 3 ranges mode Accuracy: ±0.03 Hz (50, 60 Hz), ±0.1 Hz (400 Hz range) Measurement range: 40 k-counts f.s. to 20 M-counts f.s. 6 ranges Integration mode Accuracy: ±0.0025% f.s. Measurement range: Between 10 Hz to 100 kHz (minimum pulse width 2  $\mu$ s), 100% f.s. Accuracy: ±1% (10 to 10 kHz), ±4% (10 k to 100 kHz) Duty ratio mode Measurement range: Between 2 µs to 2 s, 10 ms to 2 s f.s Pulse width mode Accuracy: ±0.1% f.s. 0.0025% f.s. (Integration mode), 0.01% f.s. (exclude integration, power Measurement resolution requency mode),0.01 Hz (power frequency mode) Input voltage range ±10 V to ±400 V, 6 ranges, selectable threshold level at each range and threshold level Slope, Level, Hold, Smoothing, Low-pass filter, Switchable DC/AC input Other functions coupling, Frequency dividing, Integration over-range keep/return

## System Chart of Options

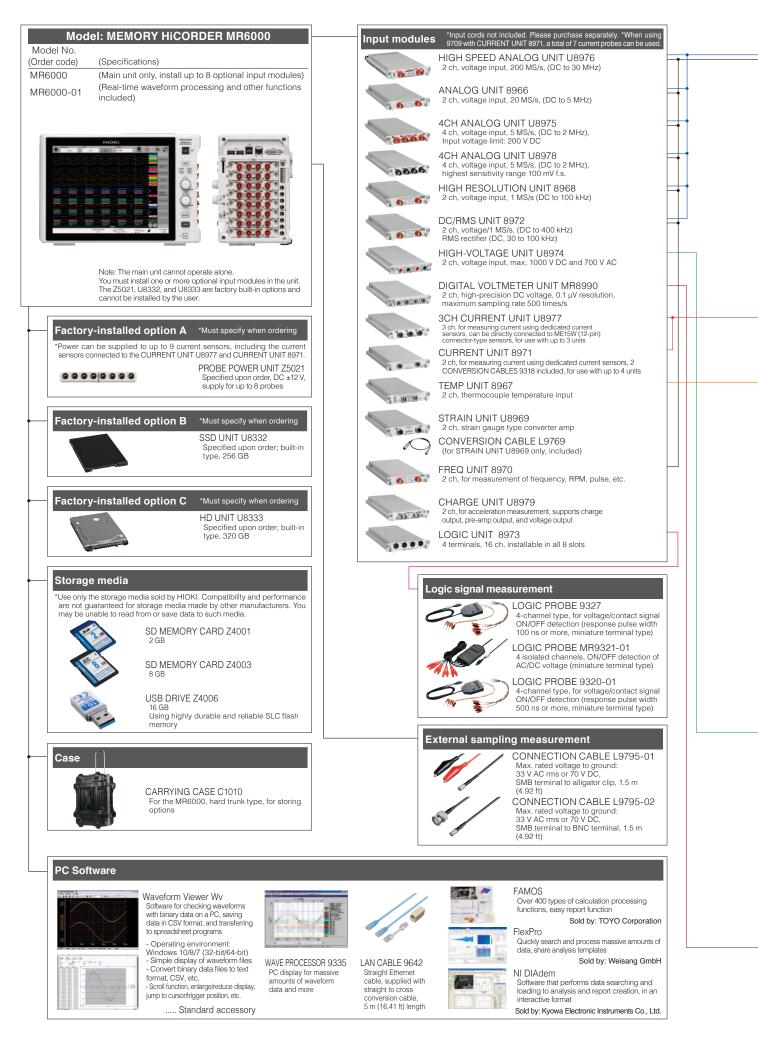

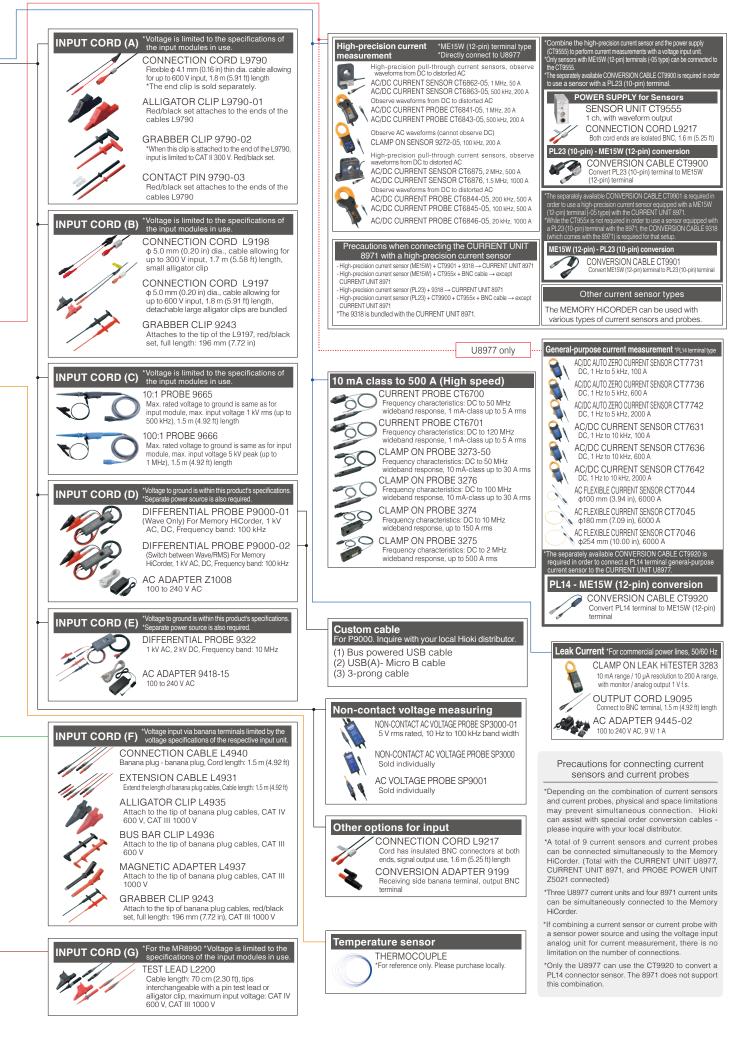

# **R&D** Tests and Critical Analyses Meeting the High Demands of a Broad Range of Industries







#### High-speed 200 MS/s measurement of inverter waveforms

Perform high-speed isolated recording across 16 channels at 200 MS/s by installing 8 units of U8976.

MEMORY HICORDER	MR6000	1 unit
HIGH SPEED ANALOG UNIT	U8976	8
10:1 PROBE	9665	16

Example configurations

MR6000E3-92E Printed in Japan

## Multi-channel measurement for ECU development

Perform multi-channel recording across 32 channels at 5 MS/s by installing 8 units of U8975.

MEMORY HICORDER	MR6000	1 unit
4ch ANALOG UNIT	U8975	8
CONNECTION CORD	L9790	32
ALLIGATOR CLIP	L9790-01	32

Perform mixed multi-channel measurements across 16 analog and 64 logic channels by installing 4 units of U8975 and 4 units of 8973.

MEMORY HICORDER	MR6000	1 unit
4ch ANALOG UNIT	U8975	4
CONNECTION CORD	L9790	16
ALLIGATOR CLIP	L9790-01	16
LOGIC UNIT	8973	4
LOGIC PROBE	9327	16

### Remove harmonic noise

The MR6000-01 comes with a digital filter calculation function that removes specific frequency noise from measurement data.

MEMORY HICORDER	MR6000-01	1 unit
ANALOG UNIT	8966	8
CONNECTION CORD	L9790	16
ALLIGATOR CLIP	L9790-01	16



#### HIOKI E.E. CORPORATION

HEADQUARTERS

81 Koizumi Ueda, Nagano 386-1192 Japan www.hioki.com

HIOKI USA CORPORATION TEL +1-609-409-9109 FAX +1-609-409-9108 hioki@hiokiusa.com / www.hiokiusa.com

All information correct as of Feb. 21, 2019. All specifications are subject to change without notice.

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies

HIOKI (Shanghai) SALES & TRADING CO., LTD. TEL +86-21-6391-0090/0092 FAX +86-21-6391-0360 info@hioki.com.cn / www.hioki.cn HIOKI SINGAPORE PTE.LTD. TEL +65-6634-7677 FAX +65-6634-7477 info-sg@hioki.com.sg / www.hioki.com.sg HIOKI KOREA CO., LTD. TEL +82-2-2183-8847 FAX +82-2-2183-3360 info-kr@hioki.co.jp / www.hiokikorea.com HIOKI EUROPE GmbH TEL +49-6173-31856-0 FAX +49-6173-31856-25 hioki@hioki.eu / www.hioki.com

HIOKI TAIWAN CO., LTD. TEL +886-3-3467160 FAX +886-3-3467162 info-tw@hioki.com.tw / www.hioki.com

DISTRIBUTED BY